

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100725AL\
Data File : FF016535.D
Signal(s) : FID2B.ch
Acq On : 07 Oct 2025 11:02
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Oct 08 02:39:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100225.M
Quant Title : GC Extractables
QLast Update : Fri Oct 03 05:49:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.978	61701	0.512 ug/ml
19) T	n-Tetratriacontane (C34)	19.766	16350	0.150 ug/ml
20) T	n-Hexatriacontane (C36)	20.559	29501	0.316 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100725AL\
Data File : FF016535.D
Signal(s) : FID2B.ch
Acq On : 07 Oct 2025 11:02
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Oct 08 02:39:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100225.M
Quant Title : GC Extractables
QLast Update : Fri Oct 03 05:49:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

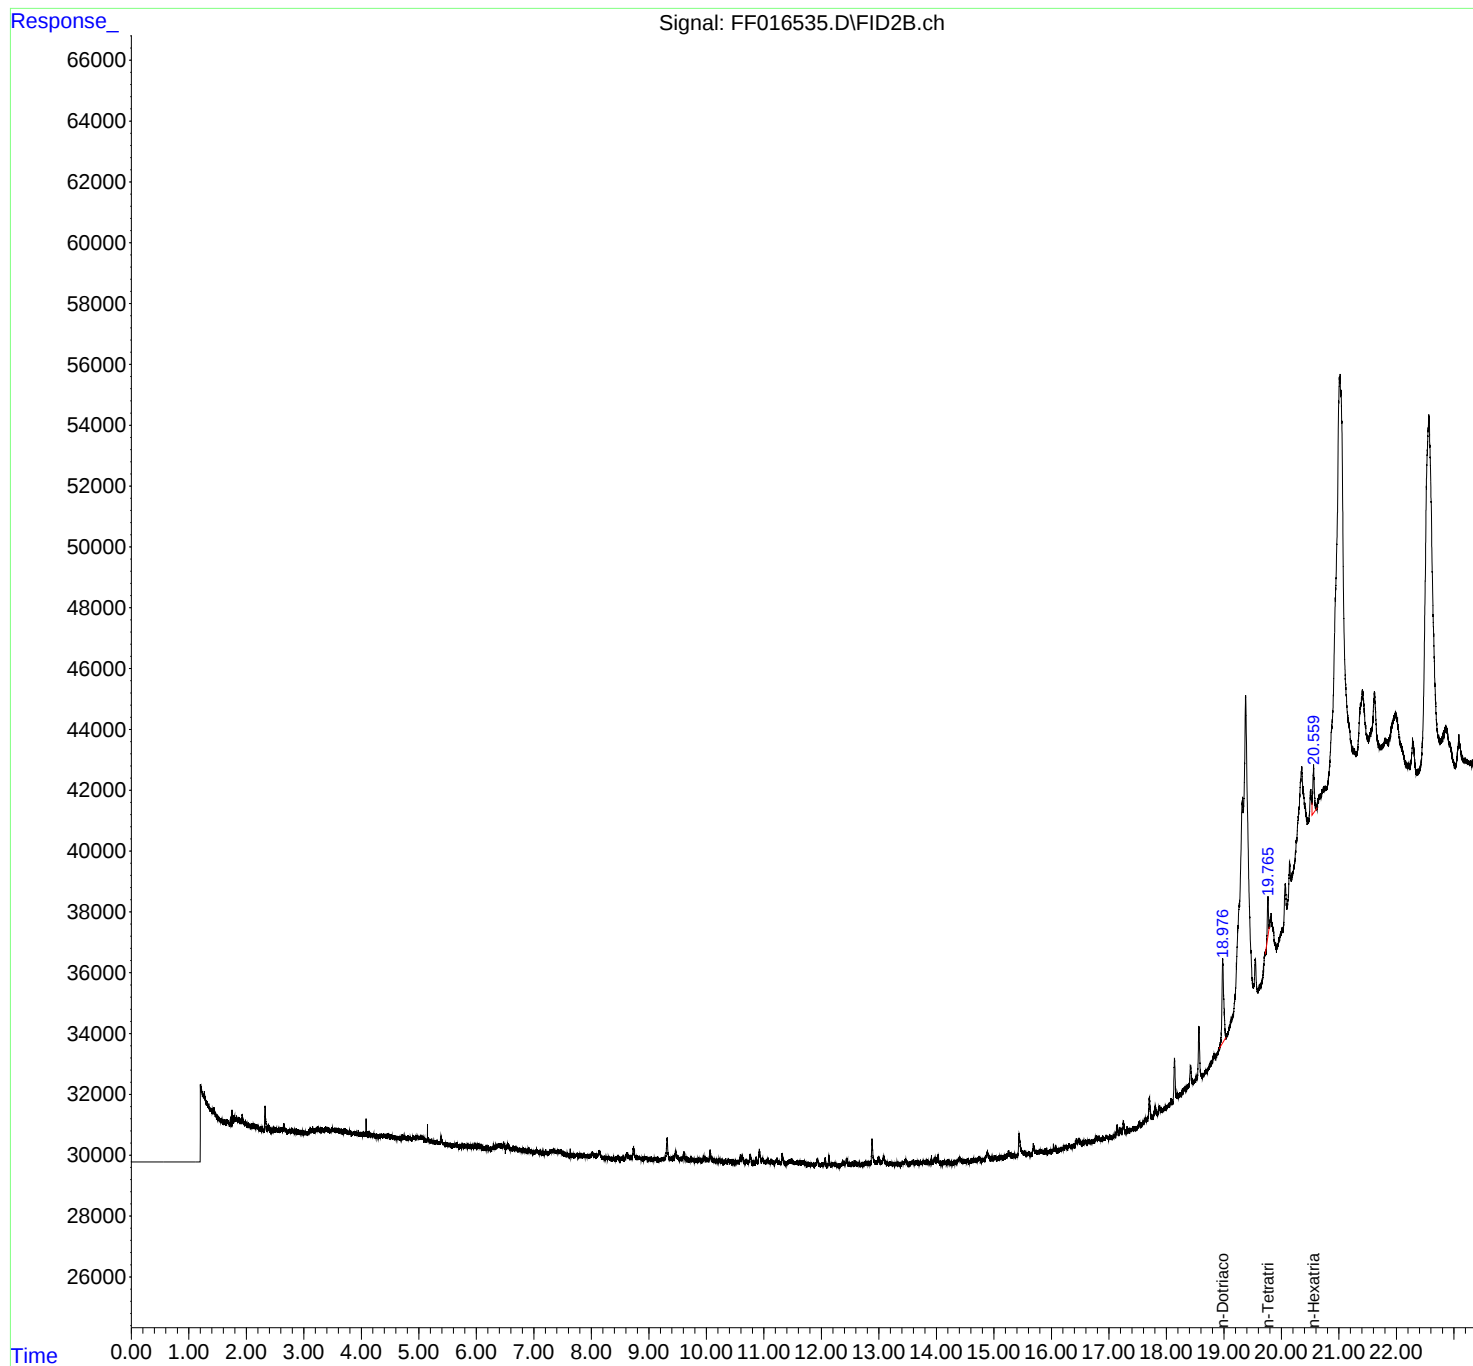


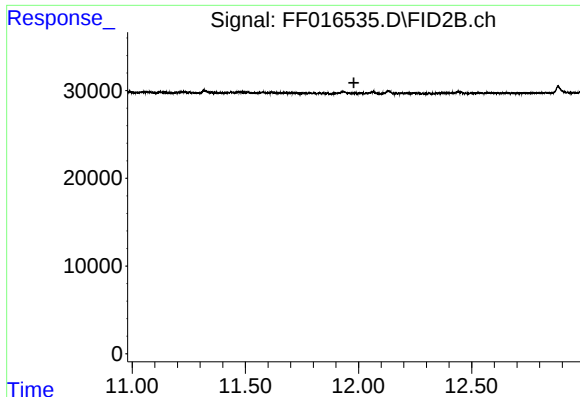

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.980 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

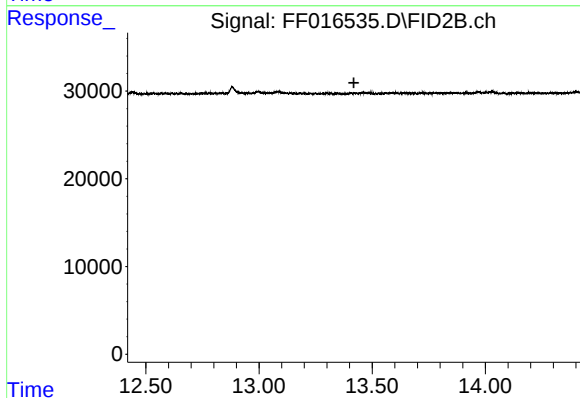


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.419 min
Response: 0
Conc: N.D.

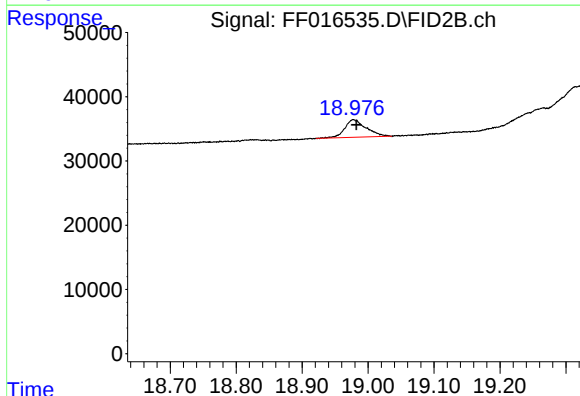


#18 n-Dotriacontane (C32)

R.T.: 18.978 min
Delta R.T.: -0.004 min
Response: 61701
Conc: 0.51 ug/ml

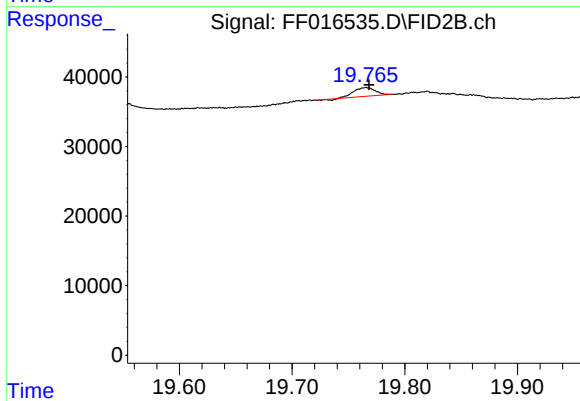

#19 n-Tetratriacontane (C34)

R.T.: 19.766 min
Delta R.T.: -0.003 min
Response: 16350
Conc: 0.15 ug/ml

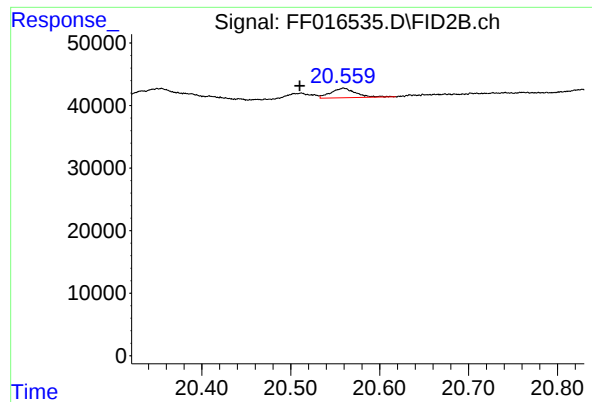

#20 n-Hexatriacontane (C36)

R.T.: 20.559 min
Delta R.T.: 0.049 min
Response: 29501
Conc: 0.32 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2