

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100821\
 Data File : FE034405.D
 Signal(s) : FID1B.CH
 Acq On : 08 Oct 2021 17:16
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 08 22:57:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
 Quant Title :
 QLast Update : Fri Oct 08 16:08:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.397	7976400	20.892 ug/ml
12) N-OCTACOSANE	16.792	8078843	21.401 ug/ml
13) N-TRIACONTANE	17.672	681383	1.828 ug/ml
14) N-DOTRIACONTANE	18.502	936657	2.615 ug/ml
15) N-TETRATRIACONTANE	19.282	712952	2.133 ug/ml
16) N-HEXATRIACONTANE	20.020	453000	1.500 ug/ml
17) N-OCTATRIACONTANE	20.743	289959	1.057 ug/ml
18) N-TETRACONTANE	21.626	178653	0.678 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100821\
Data File : FE034405.D
Signal(s) : FID1B.CH
Acq On : 08 Oct 2021 17:16
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 22:57:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
Quant Title :
QLast Update : Fri Oct 08 16:08:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

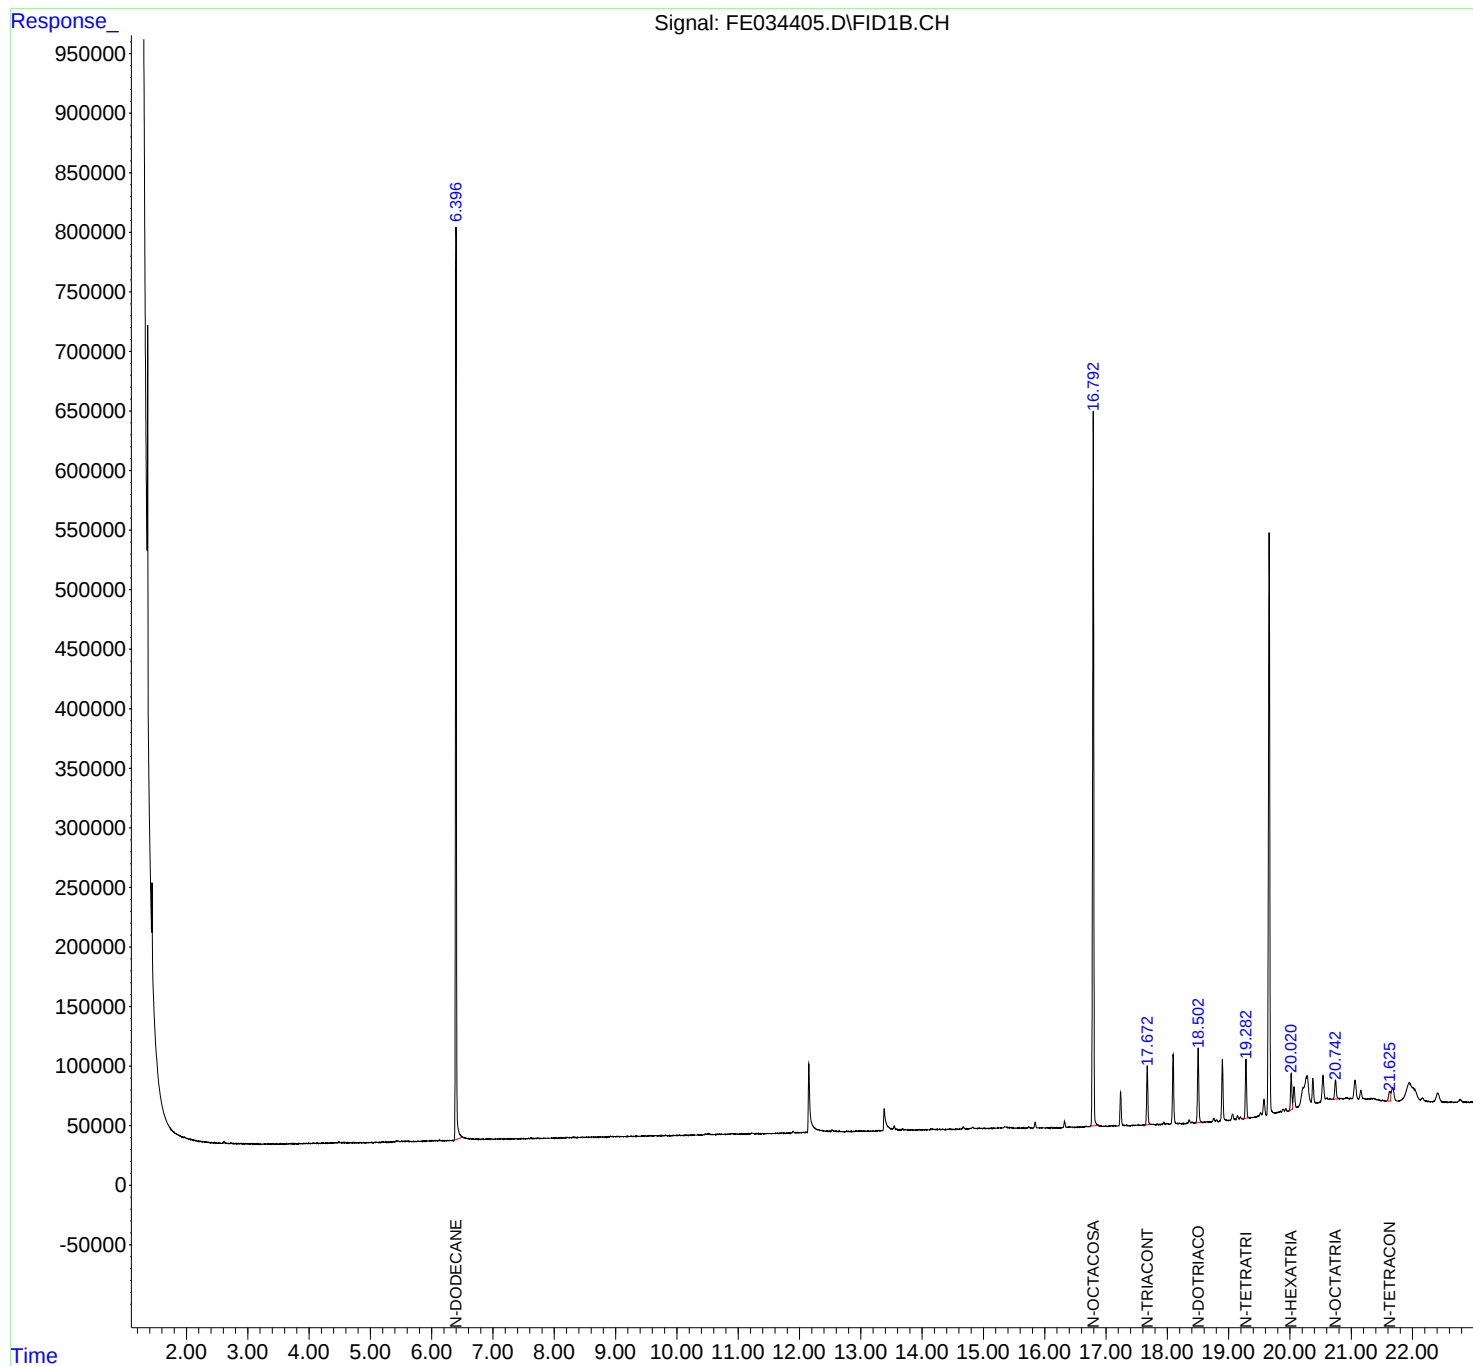


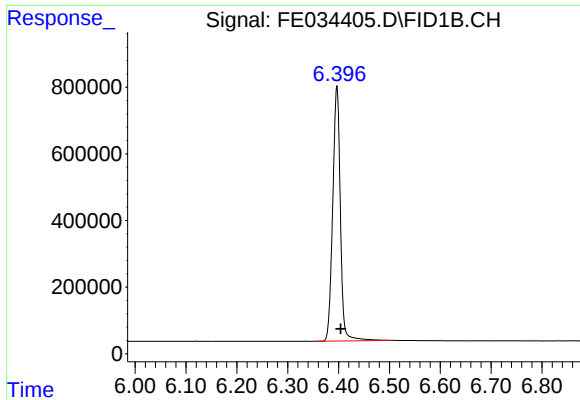

#3 N-DODECANE


R.T.: 6.397 min
Delta R.T.: -0.007 min
Response: 7976400
Conc: 20.89 ug/ml

Instrument :
FID_E
ClientSampleId :

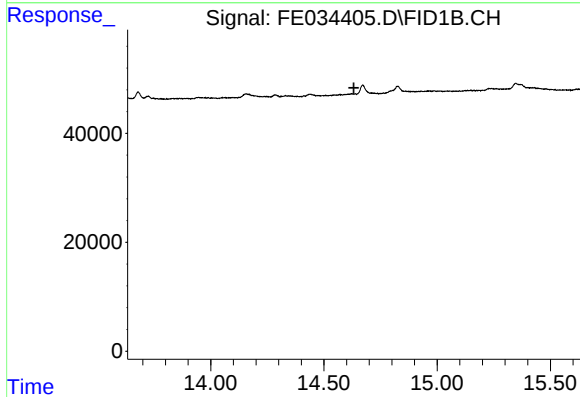


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.632 min
Response: 0
Conc: N.D.

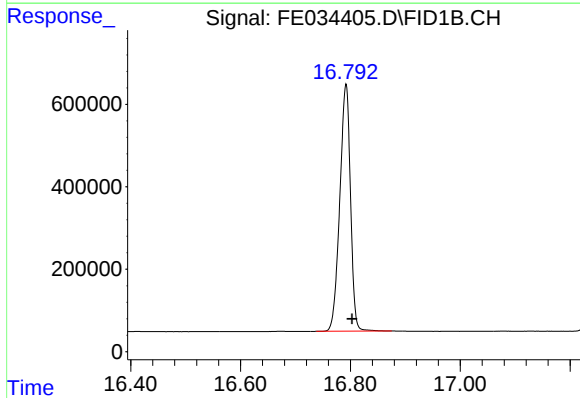


#12 N-OCTACOSANE

R.T.: 16.792 min
Delta R.T.: -0.011 min
Response: 8078843
Conc: 21.40 ug/ml

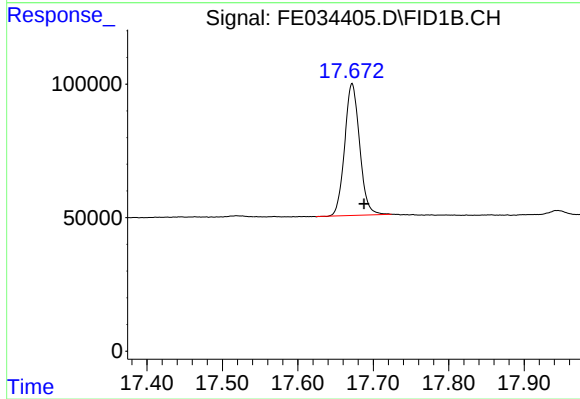

#13 N-TRIACONTANE


R.T.: 17.672 min
Delta R.T.: -0.016 min
Response: 681383
Conc: 1.83 ug/ml

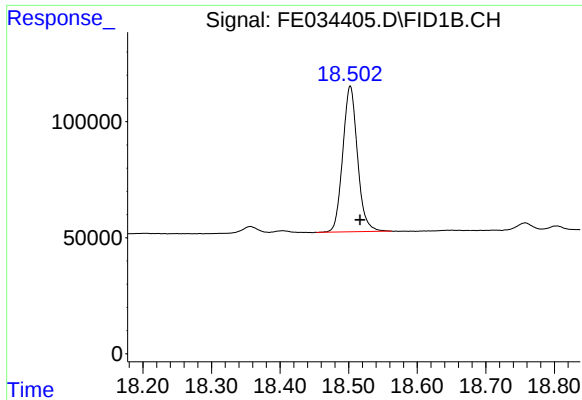

#14 N-DOTRIACONTANE


R.T.: 18.502 min
Delta R.T.: -0.014 min
Response: 936657
Conc: 2.62 ug/ml

Instrument :
FID_E
ClientSampleId :

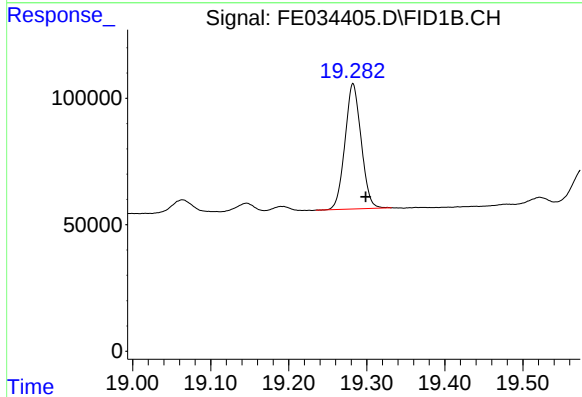


#15 N-TETRATRIACONTANE

R.T.: 19.282 min
Delta R.T.: -0.016 min
Response: 712952
Conc: 2.13 ug/ml

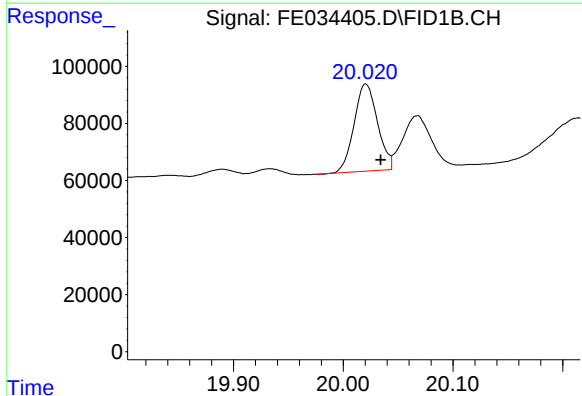


#16 N-HEXATRIACONTANE

R.T.: 20.020 min
Delta R.T.: -0.014 min
Response: 453000
Conc: 1.50 ug/ml

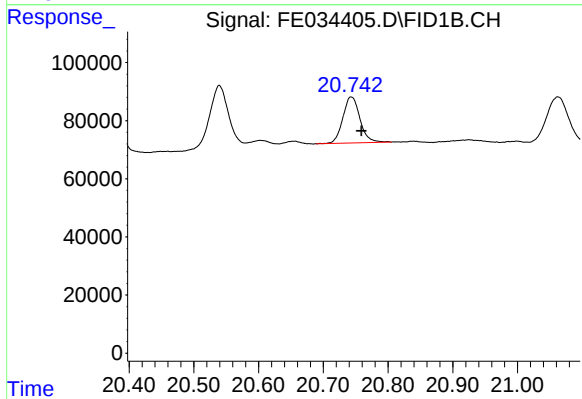

#17 N-OCTATRIACONTANE

R.T.: 20.743 min
Delta R.T.: -0.016 min
Response: 289959
Conc: 1.06 ug/ml

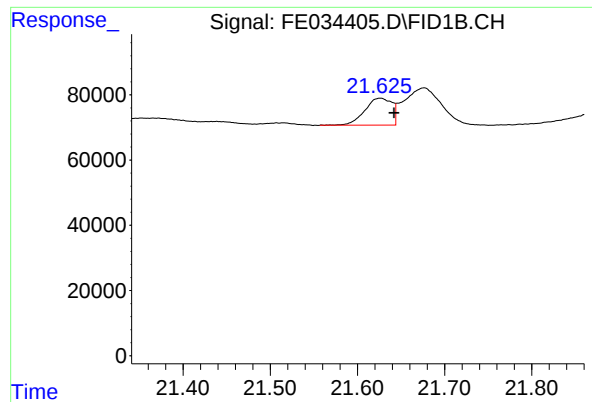

#18 N-TETRACONTANE

R.T.: 21.626 min
Delta R.T.: -0.015 min
Response: 178653
Conc: 0.68 ug/ml

Instrument :
FID_E
ClientSampleId :