

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100821\
Data File : FE034409.D
Signal(s) : FID1B.CH
Acq On : 08 Oct 2021 19:36
Operator : DD\AJ
Sample : M4144-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 22:58:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
Quant Title :
QLast Update : Fri Oct 08 16:08:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.618	207479	0.608 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100821\
Data File : FE034409.D
Signal(s) : FID1B.CH
Acq On : 08 Oct 2021 19:36
Operator : DD\AJ
Sample : M4144-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 08 22:58:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
Quant Title :
QLast Update : Fri Oct 08 16:08:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

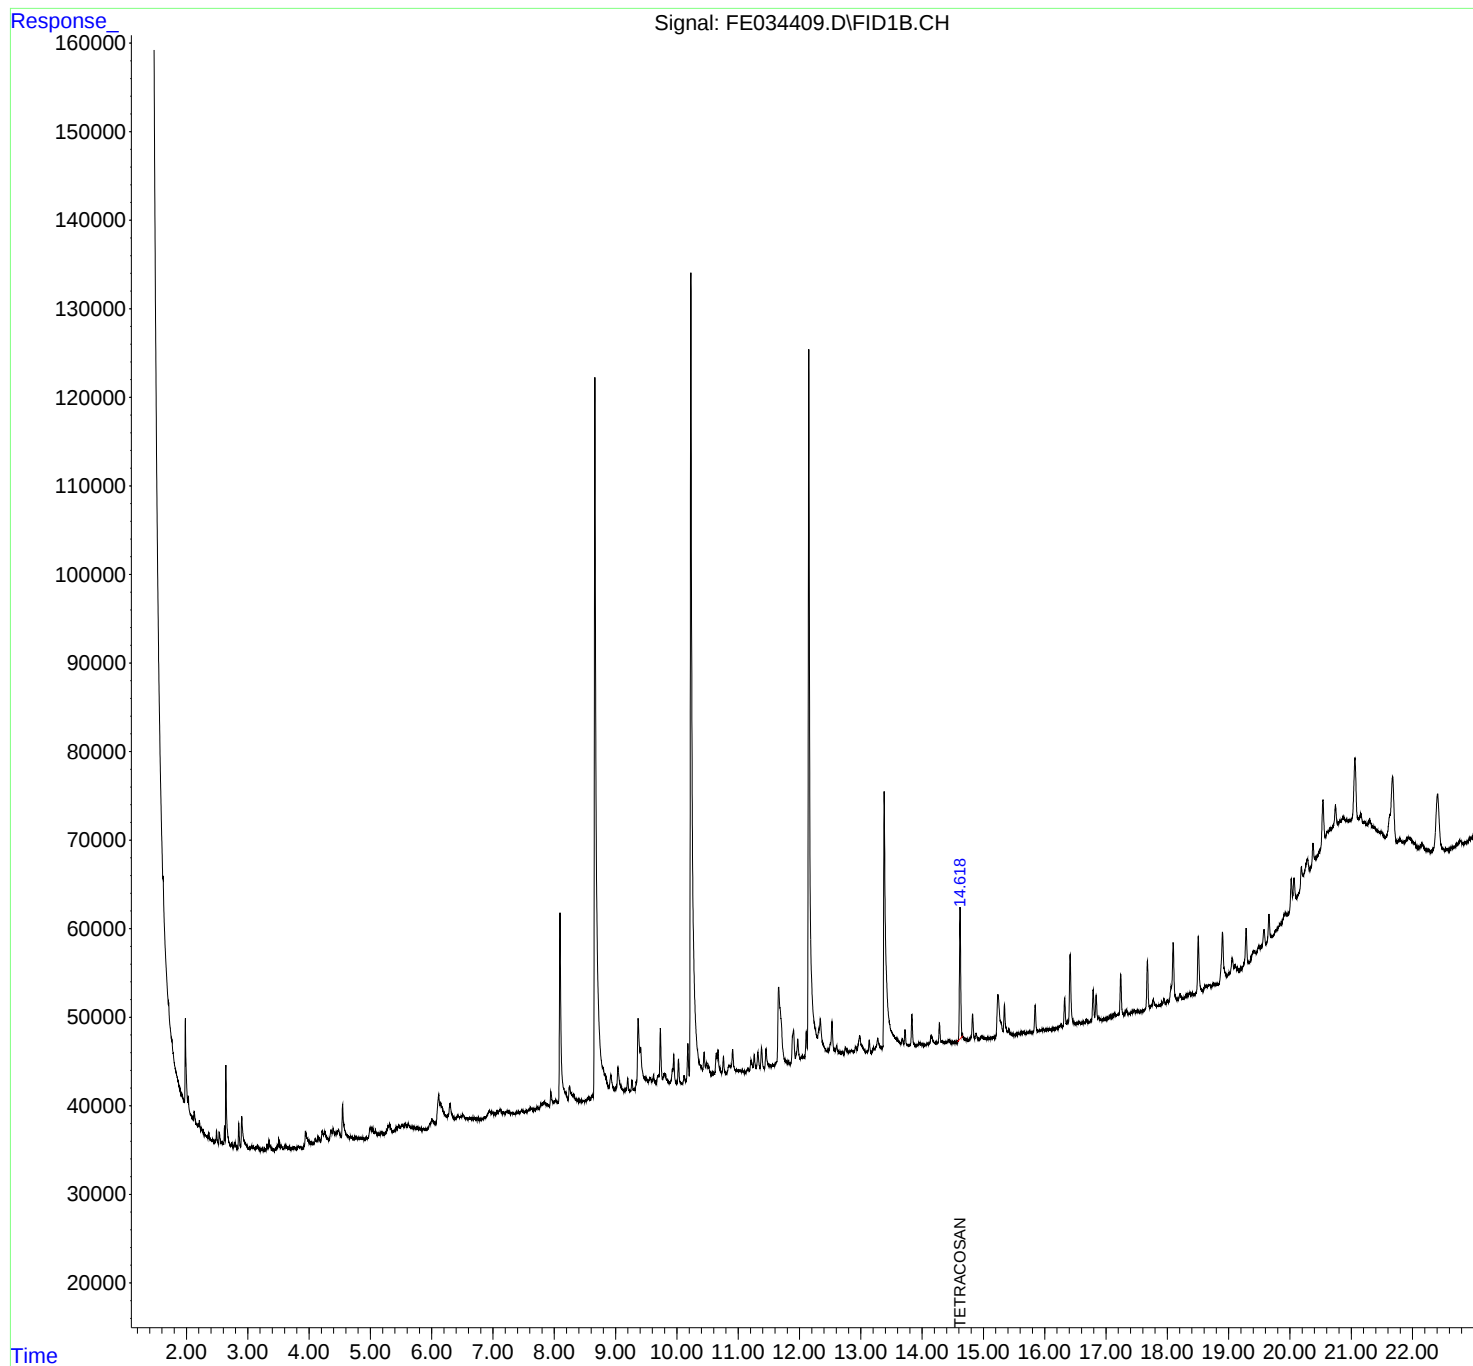

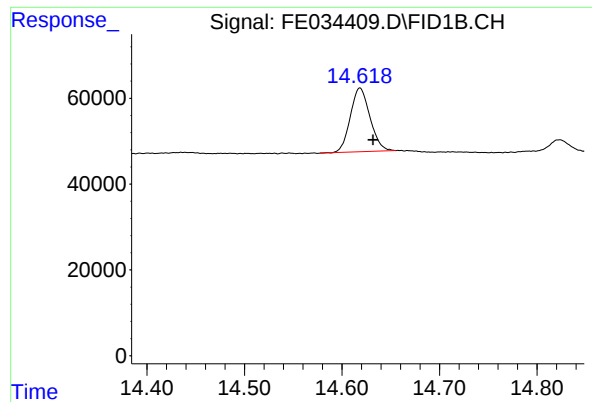

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.618 min
Delta R.T.: -0.013 min
Response: 207479
Conc: 0.61 ug/ml

Instrument :
FID_E
ClientSampleId :