

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100821\
 Data File : FE034404.D
 Signal(s) : FID1B.CH
 Acq On : 08 Oct 2021 16:41
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Oct 08 23:04:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
 Quant Title :
 QLast Update : Fri Oct 08 16:08:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.631	17562196	51.502 ug/ml
Target Compounds			
2) N-DECANE	4.397	20193478	52.564 ug/ml
3) N-DODECANE	6.404	20412677	53.466 ug/ml
4) N-TETRADECANE	8.195	20678170	52.555 ug/ml
5) N-HEXADECANE	9.793	20492645	51.885 ug/ml
6) N-OCTADECANE	11.232	20717920	51.620 ug/ml
7) N-EICOSANE	12.540	20629604	51.275 ug/ml
8) N-DOCOSANE	13.736	20235022	51.488 ug/ml
10) N-TETRACOSANE	14.836	20081314	51.569 ug/ml
11) N-HEXACOSANE	15.854	19748531	51.766 ug/ml
12) N-OCTACOSANE	16.801	19476541	51.595 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100821\
Data File : FE034404.D
Signal(s) : FID1B.CH
Acq On : 08 Oct 2021 16:41
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Oct 08 23:04:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
Quant Title :
QLast Update : Fri Oct 08 16:08:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

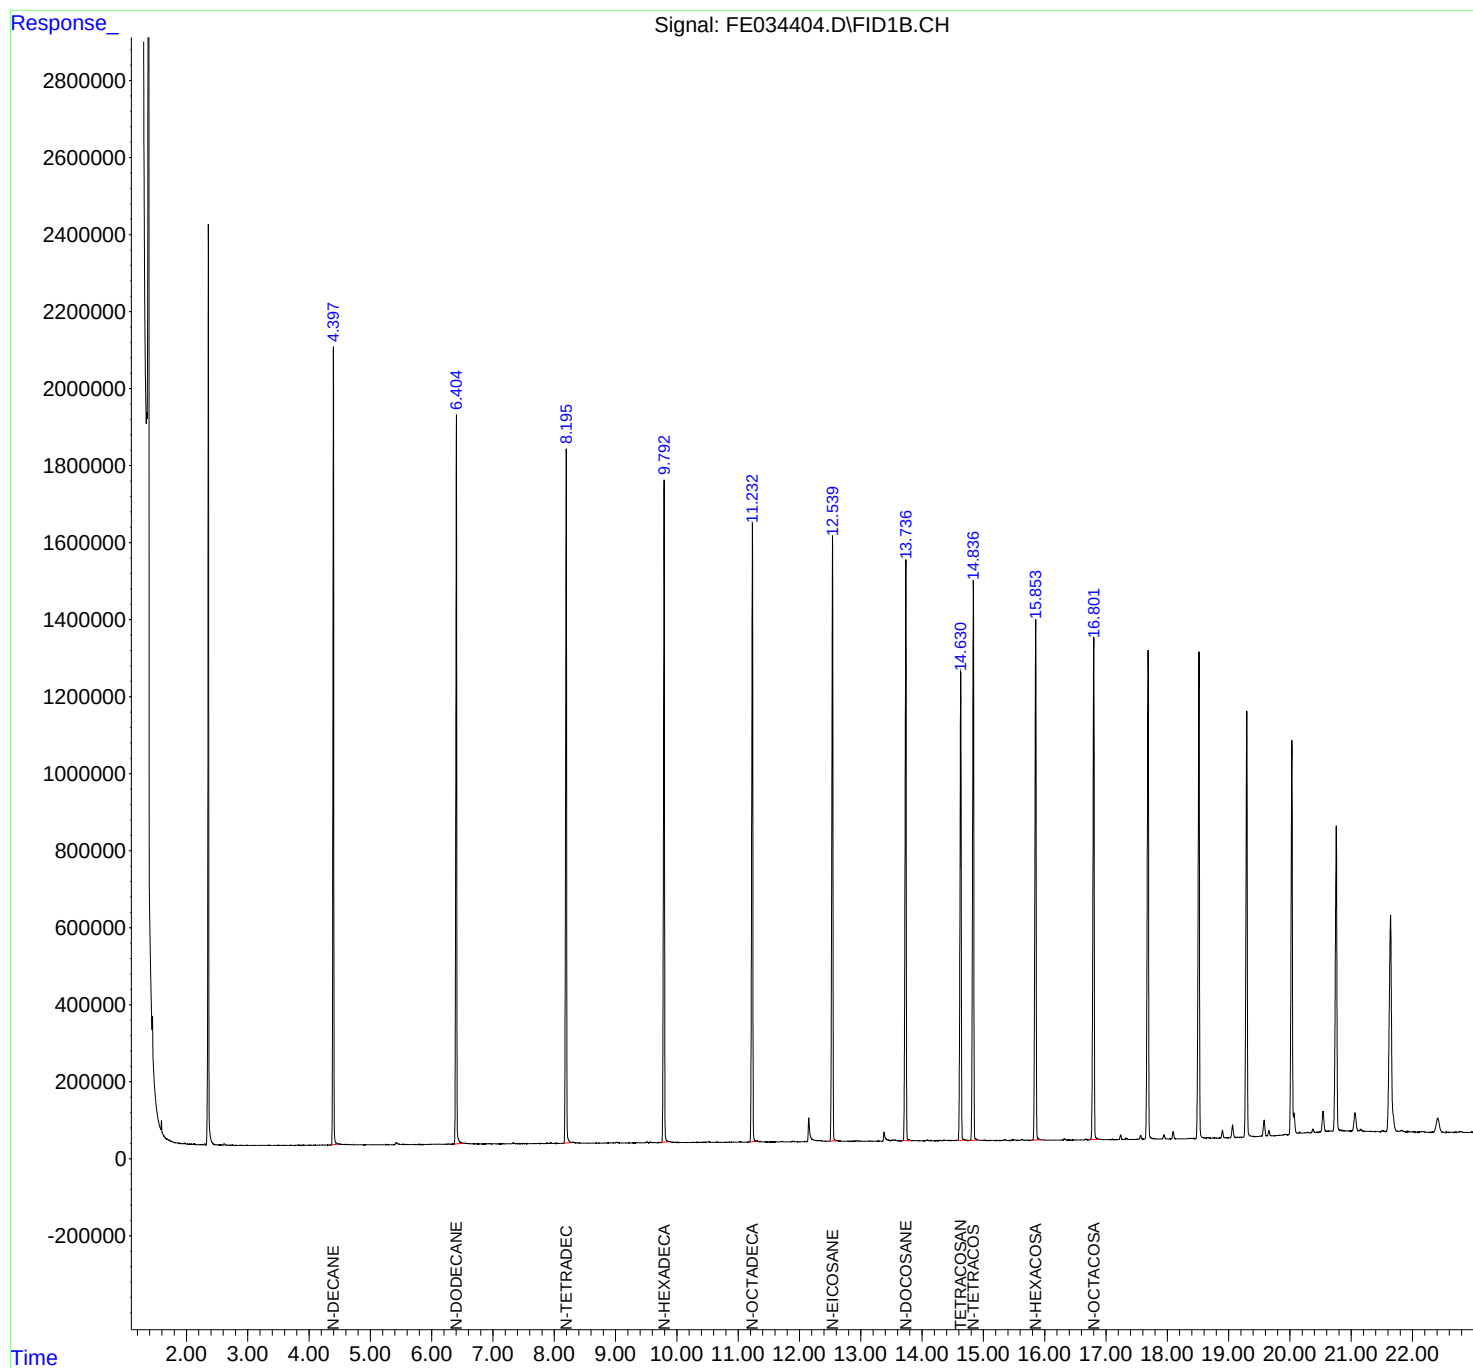


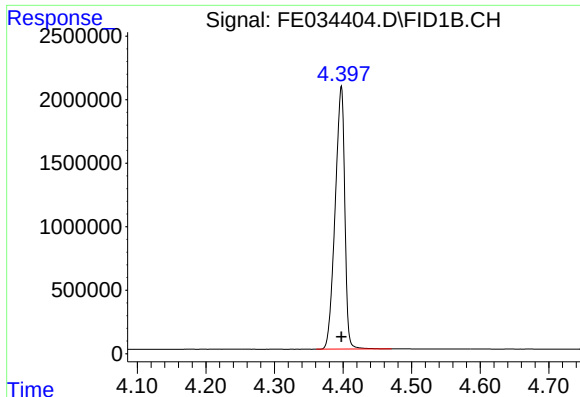

#2 N-DECANE


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 20193478
Conc: 52.56 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

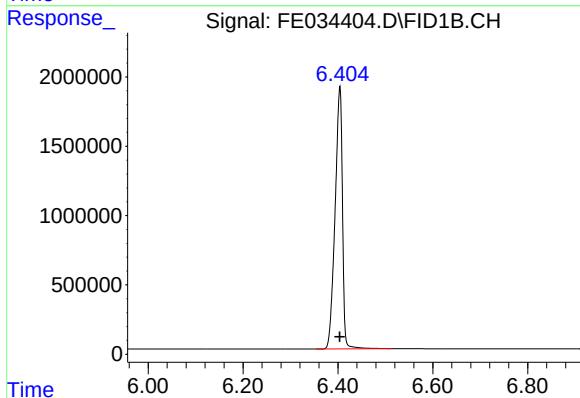


#3 N-DODECANE

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 20412677
Conc: 53.47 ug/ml

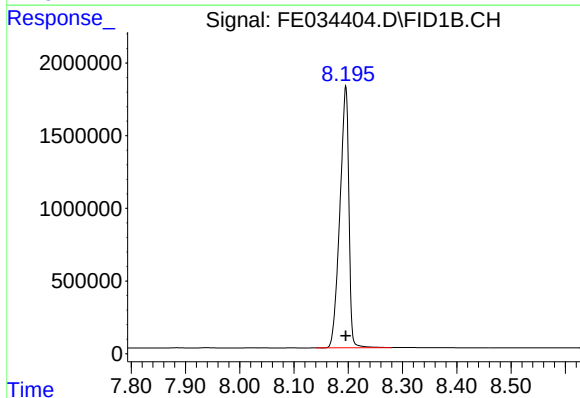


#4 N-TETRADECANE

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 20678170
Conc: 52.56 ug/ml

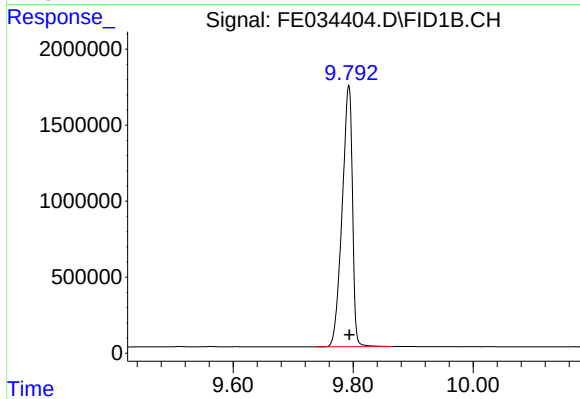

#5 N-HEXADECANE


R.T.: 9.793 min
Delta R.T.: -0.001 min
Response: 20492645
Conc: 51.88 ug/ml

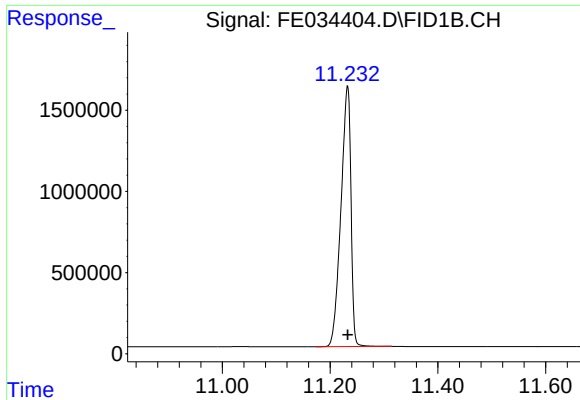

#6 N-OCTADECANE


R.T.: 11.232 min
Delta R.T.: 0.000 min
Response: 20717920
Conc: 51.62 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

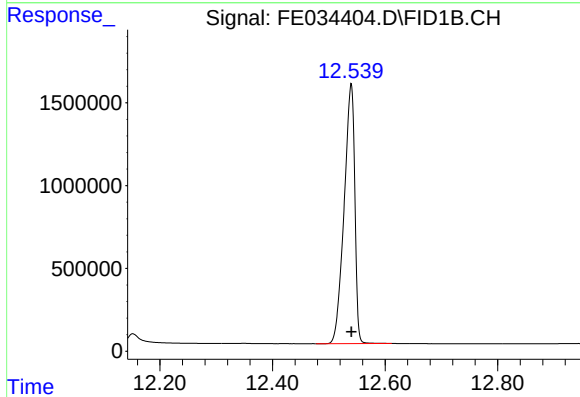


#7 N-EICOSANE

R.T.: 12.540 min
Delta R.T.: 0.000 min
Response: 20629604
Conc: 51.27 ug/ml

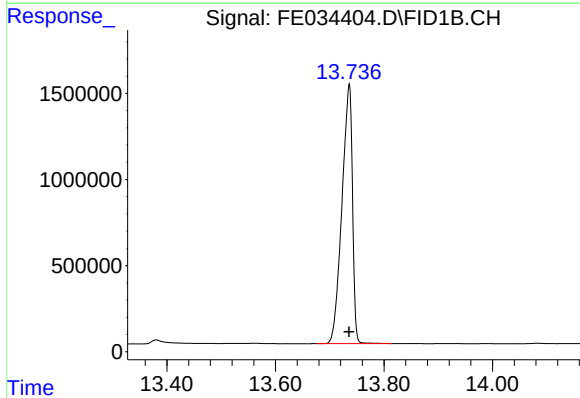


#8 N-DOCOSANE

R.T.: 13.736 min
Delta R.T.: 0.000 min
Response: 20235022
Conc: 51.49 ug/ml

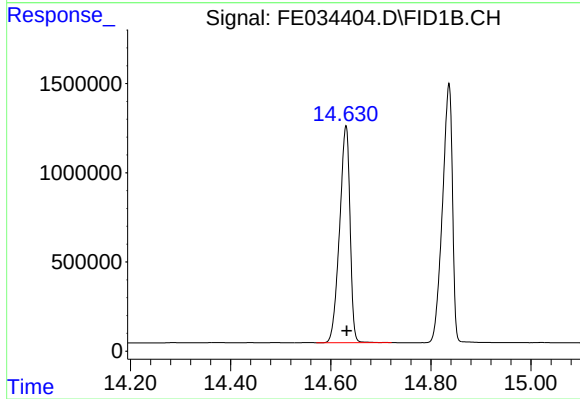

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.631 min
Delta R.T.: -0.001 min
Response: 17562196
Conc: 51.50 ug/ml

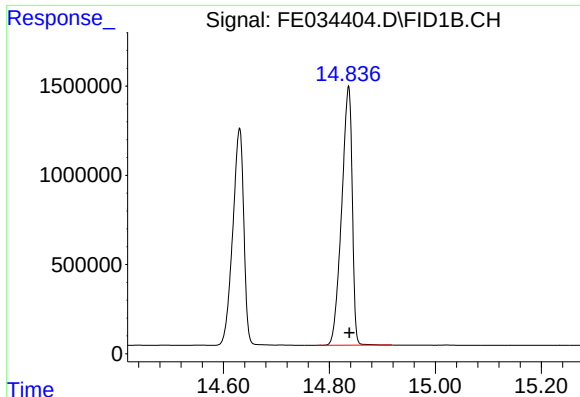

#10 N-TETRACOSANE


R.T.: 14.836 min
Delta R.T.: -0.001 min
Response: 20081314
Conc: 51.57 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

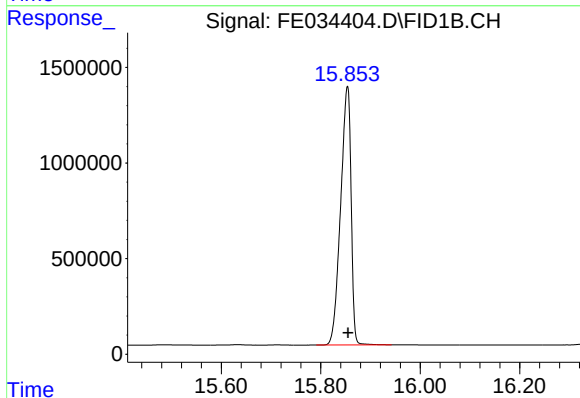

#11 N-HEXACOSANE

R.T.: 15.854 min
Delta R.T.: -0.001 min
Response: 19748531
Conc: 51.77 ug/ml

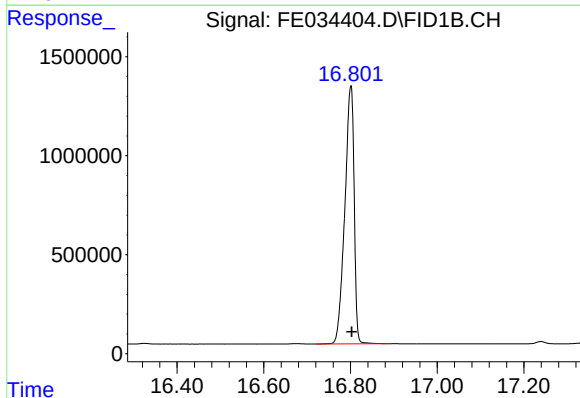

#12 N-OCTACOSANE

R.T.: 16.801 min
Delta R.T.: -0.002 min
Response: 19476541
Conc: 51.59 ug/ml