

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100821\  
 Data File : FE034411.D  
 Signal(s) : FID1B.CH  
 Acq On : 08 Oct 2021 20:46  
 Operator : DD\AJ  
 Sample : M4144-03  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 IDW-LIQ-COMP-100721

Manual Integrations  
 APPROVED

mohammad  
 10/12/2021 8:43:24 AM

Integration File: Sample.e  
 Quant Time: Oct 08 22:58:53 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE100821.M  
 Quant Title :  
 QLast Update : Fri Oct 08 16:08:59 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.627 | 6993358  | 20.509 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100821\  
Data File : FE034411.D  
Signal(s) : FID1B.CH  
Acq On : 08 Oct 2021 20:46  
Operator : DD\AJ  
Sample : M4144-03  
Misc :  
ALS Vial : 10 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
IDW-LIQ-COMP-100721


Manual Integrations  
APPROVED

mohammad  
10/12/2021 8:43:24 AM

Integration File: Sample.e  
Quant Time: Oct 08 22:58:53 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE100821.M  
Quant Title :  
QLast Update : Fri Oct 08 16:08:59 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

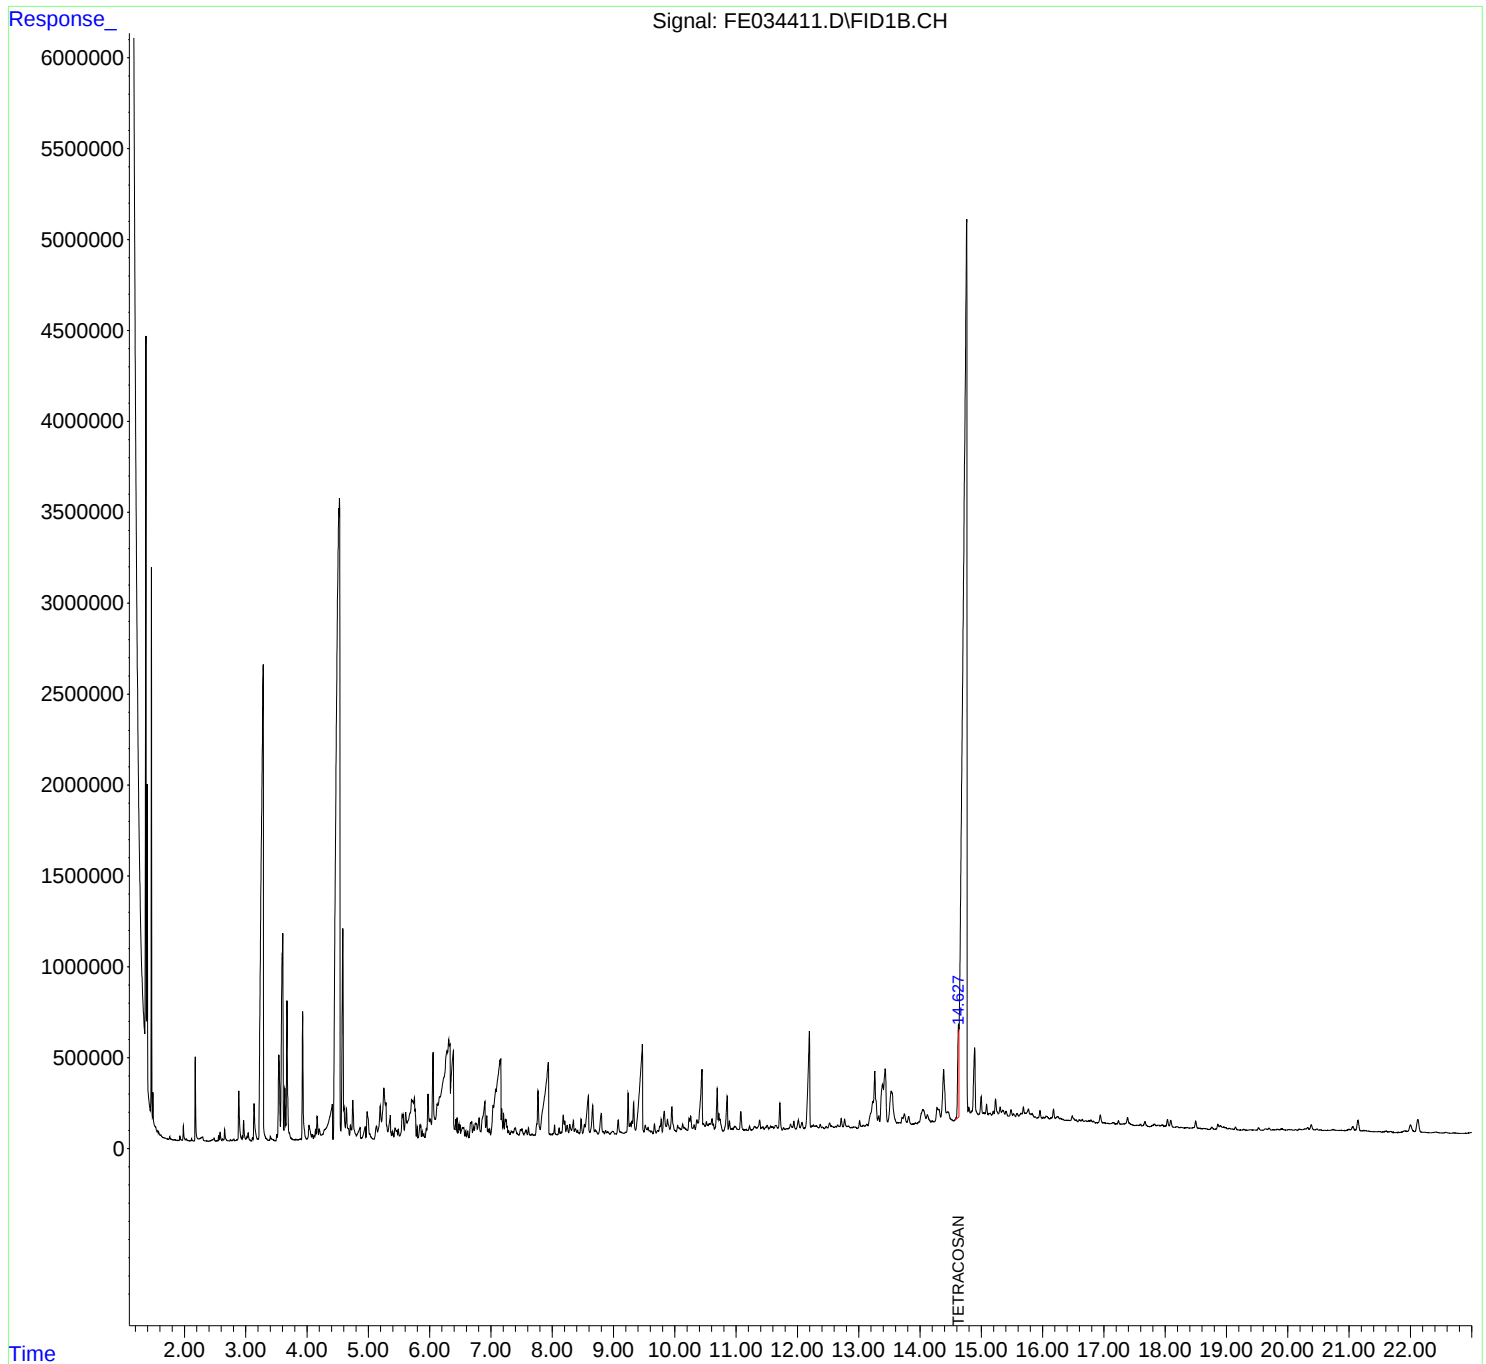

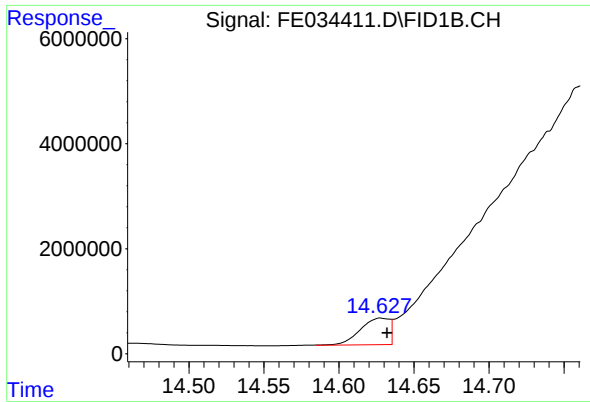

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min  
Delta R.T.: -0.005 min  
Response: 6993358  
Conc: 20.51 ug/ml m

Instrument :  
FID\_E  
ClientSampleId :  
IDW-LIQ-COMP-100721

Manual Integrations  
APPROVED  
mohammad  
10/12/2021 8:43:24 AM