

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100823\
 Data File : FE044712.D
 Signal(s) : FID1B.ch
 Acq On : 08 Oct 2023 07:25
 Operator : YP\AJ
 Sample : PB156131BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 09 00:23:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
 Quant Title :
 QLast Update : Tue Oct 03 12:58:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.013	2703921	18.430 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.080	66926	0.451 ug/ml
14) N-DOTRIACONTANE	18.914	90731	0.626 ug/ml
15) N-TETRATRIACONTANE	19.699	72536	0.567 ug/ml
16) N-HEXATRIACONTANE	20.442	47380	0.449 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100823\
Data File : FE044712.D
Signal(s) : FID1B.ch
Acq On : 08 Oct 2023 07:25
Operator : YP\AJ
Sample : PB156131BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 09 00:23:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

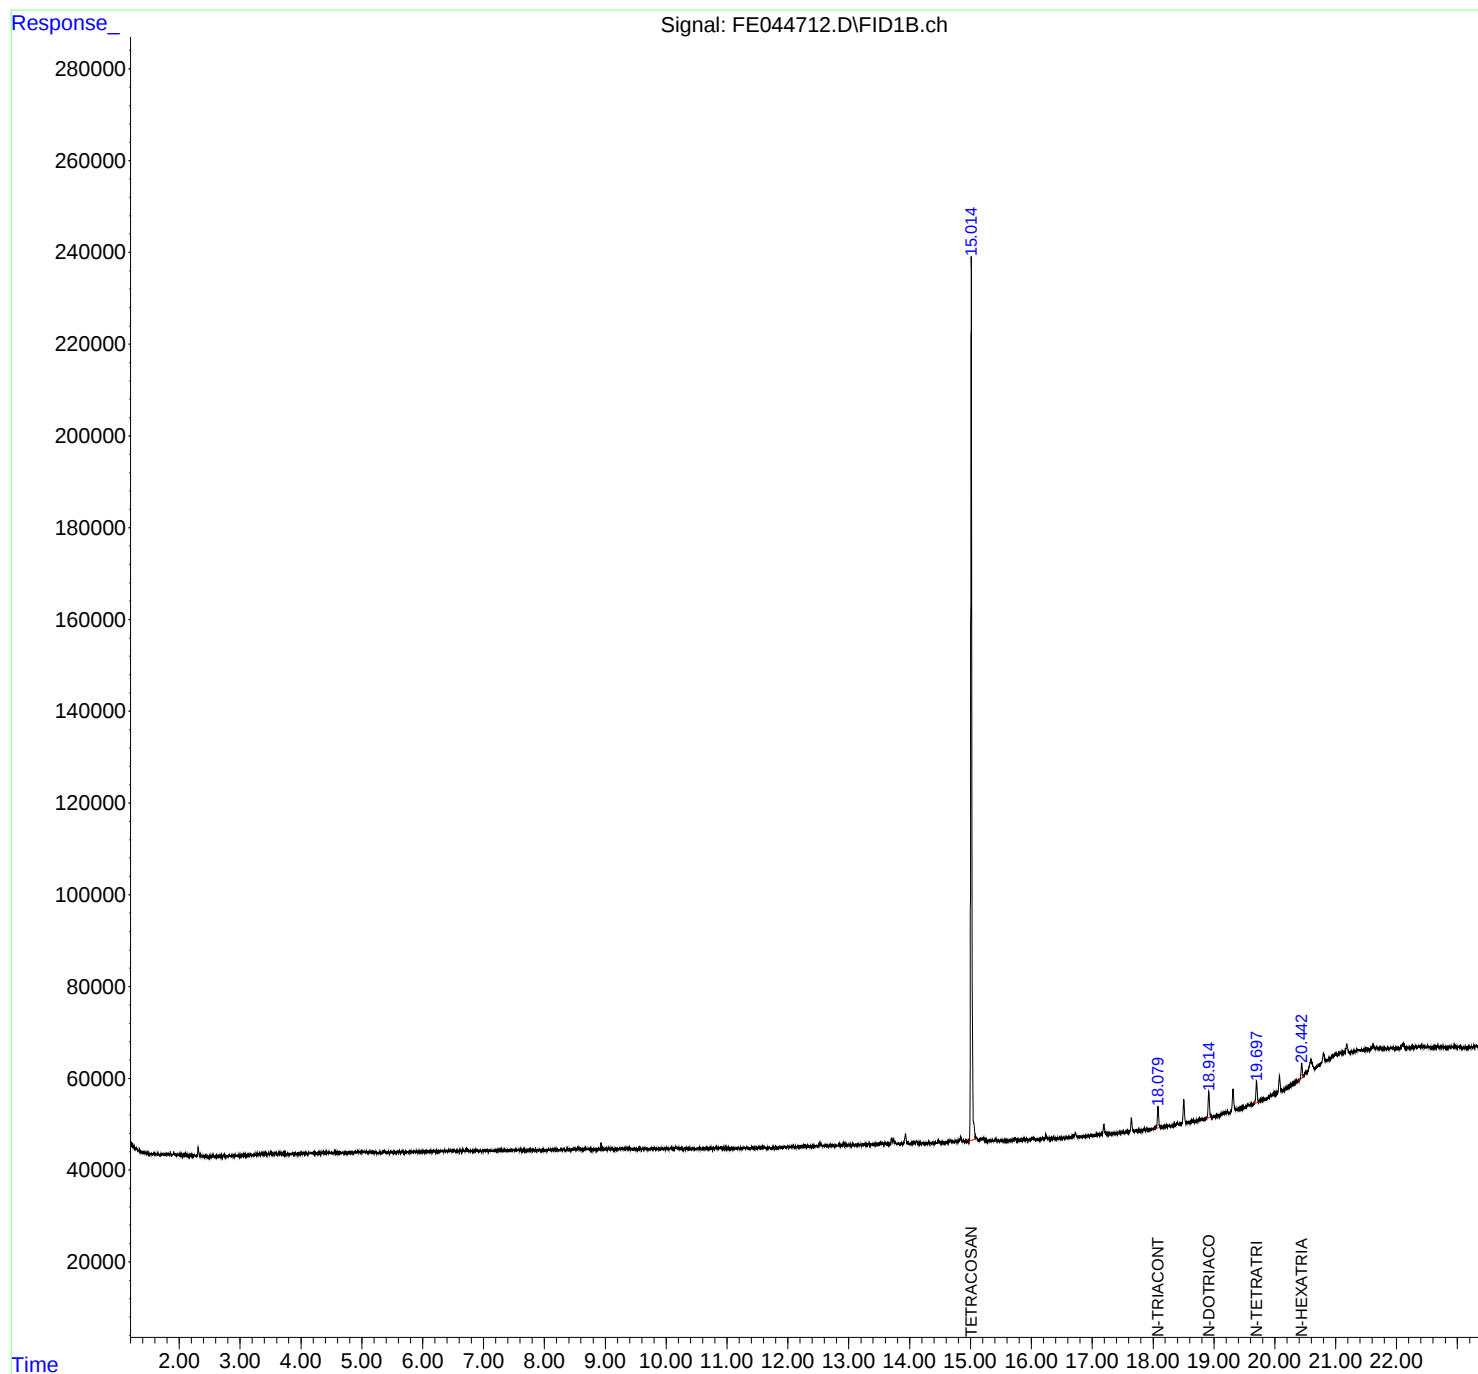

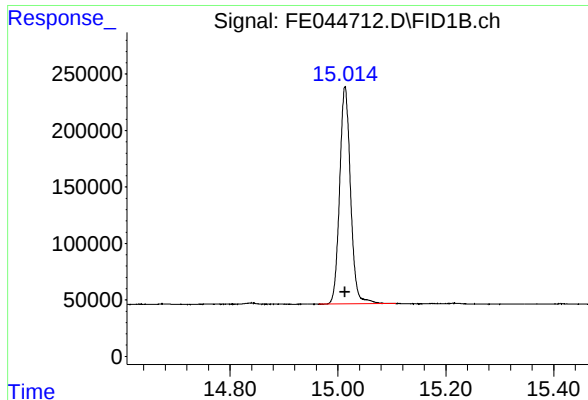


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.013 min
Delta R.T.: 0.000 min
Response: 2703921
Conc: 18.43 ug/ml

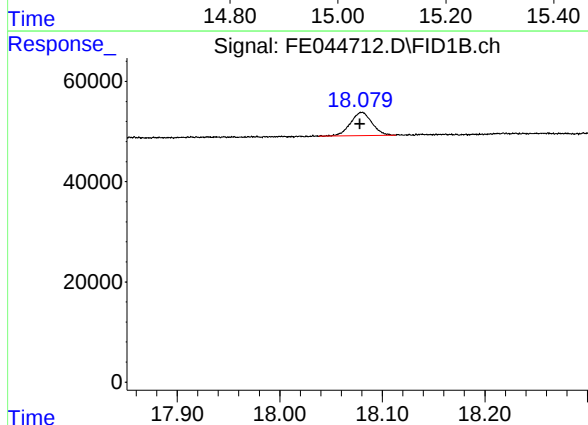


#13 N-TRIACONTANE

R.T.: 18.080 min
Delta R.T.: 0.002 min
Response: 66926
Conc: 0.45 ug/ml

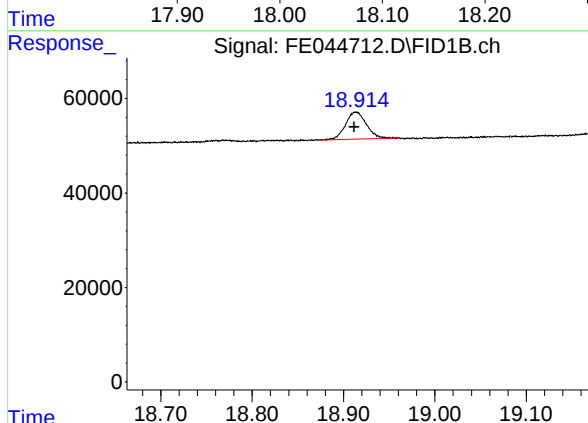


#14 N-DOTRIACONTANE

R.T.: 18.914 min
Delta R.T.: 0.002 min
Response: 90731
Conc: 0.63 ug/ml

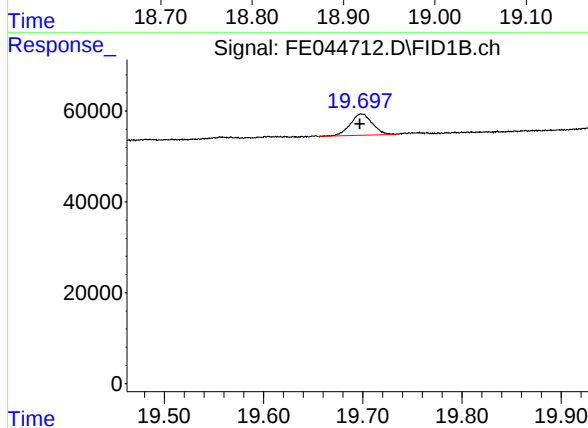

#15 N-TETRATRIACONTANE

R.T.: 19.699 min
Delta R.T.: 0.001 min
Response: 72536
Conc: 0.57 ug/ml

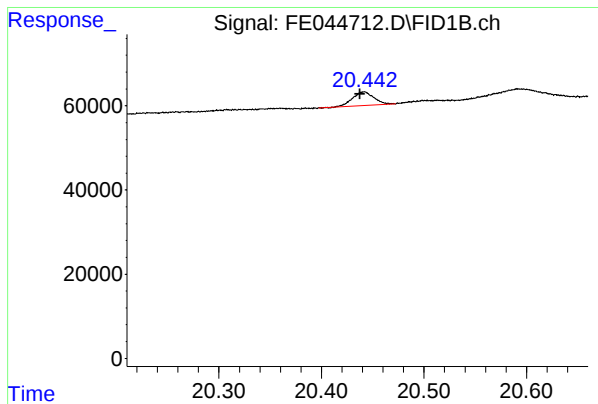

#16 N-HEXATRIACONTANE

R.T.: 20.442 min
Delta R.T.: 0.004 min
Response: 47380
Conc: 0.45 ug/ml