

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100823\
Data File : FE044709.D
Signal(s) : FID1B.ch
Acq On : 08 Oct 2023 05:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 09 00:22:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.013	2671021	18.206 ug/ml
Target Compounds			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100823\
Data File : FE044709.D
Signal(s) : FID1B.ch
Acq On : 08 Oct 2023 05:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 09 00:22:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

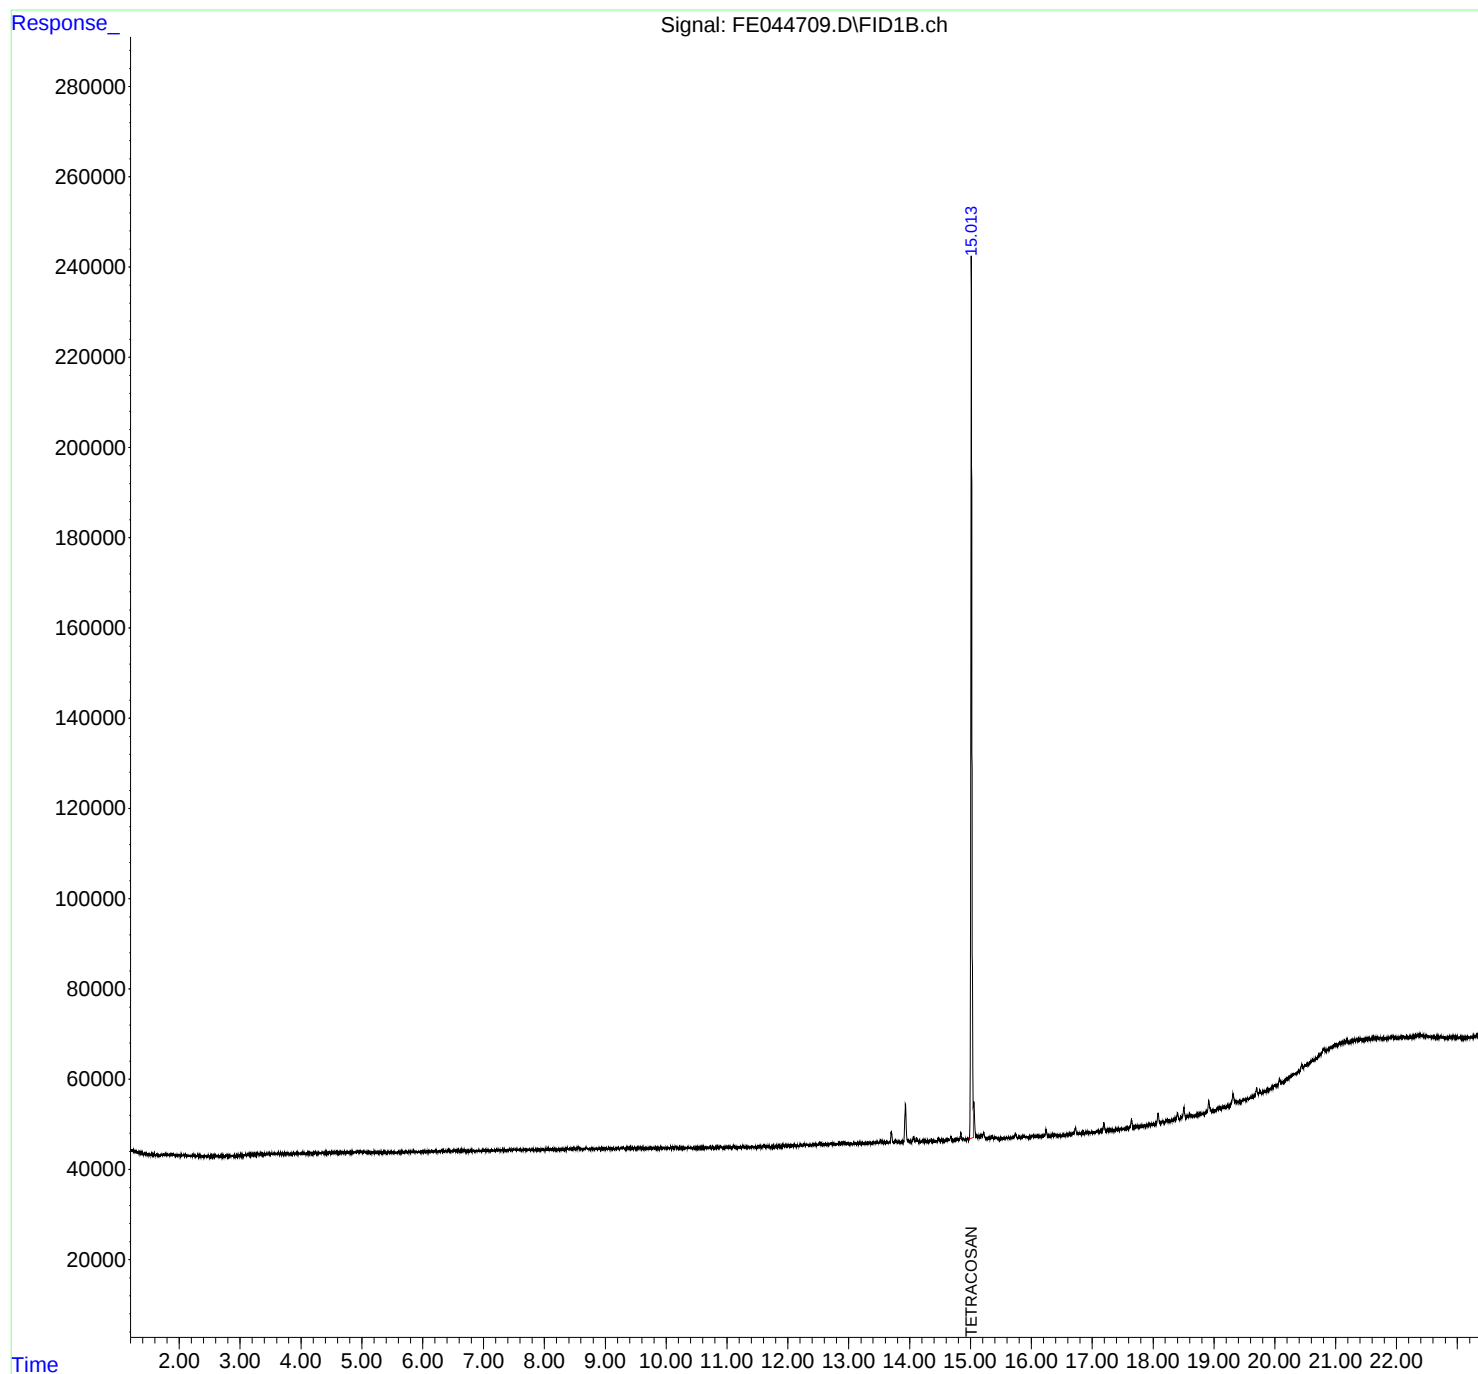

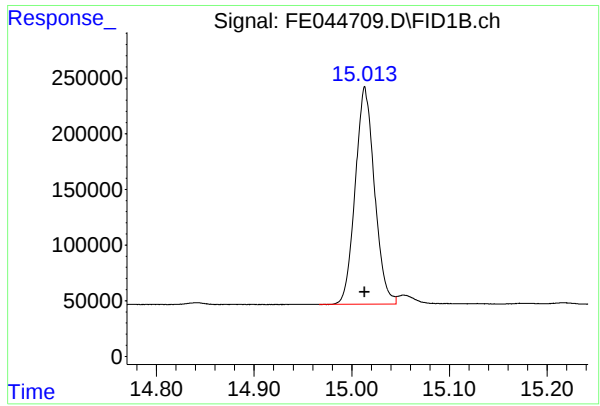

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.013 min
Delta R.T.: 0.000 min
Response: 2671021
Conc: 18.21 ug/ml