

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100825\
 Data File : FB032239.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2025 11:06
 Operator : YP/AJ
 Sample : BSF1008S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 09 04:10:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	364181	20.346 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	797639	29.535 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	920023	32.569 ng/ml
3) t n-Heptane	7.759	277011	10.138 ng/ml
4) t Benzene	7.897	338968	9.379 ng/ml
6) t Toluene	10.628	1054461	28.312 ng/ml
7) t Ethylbenzene	13.064	311205	9.520 ng/ml
8) t m-Xylene	13.197	643824	18.889 ng/ml
9) t O-Xylene	13.924	616388	18.876 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	522635	18.685 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100825\
Data File : FB032239.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2025 11:06
Operator : YP/AJ
Sample : BSF1008S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 09 04:10:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

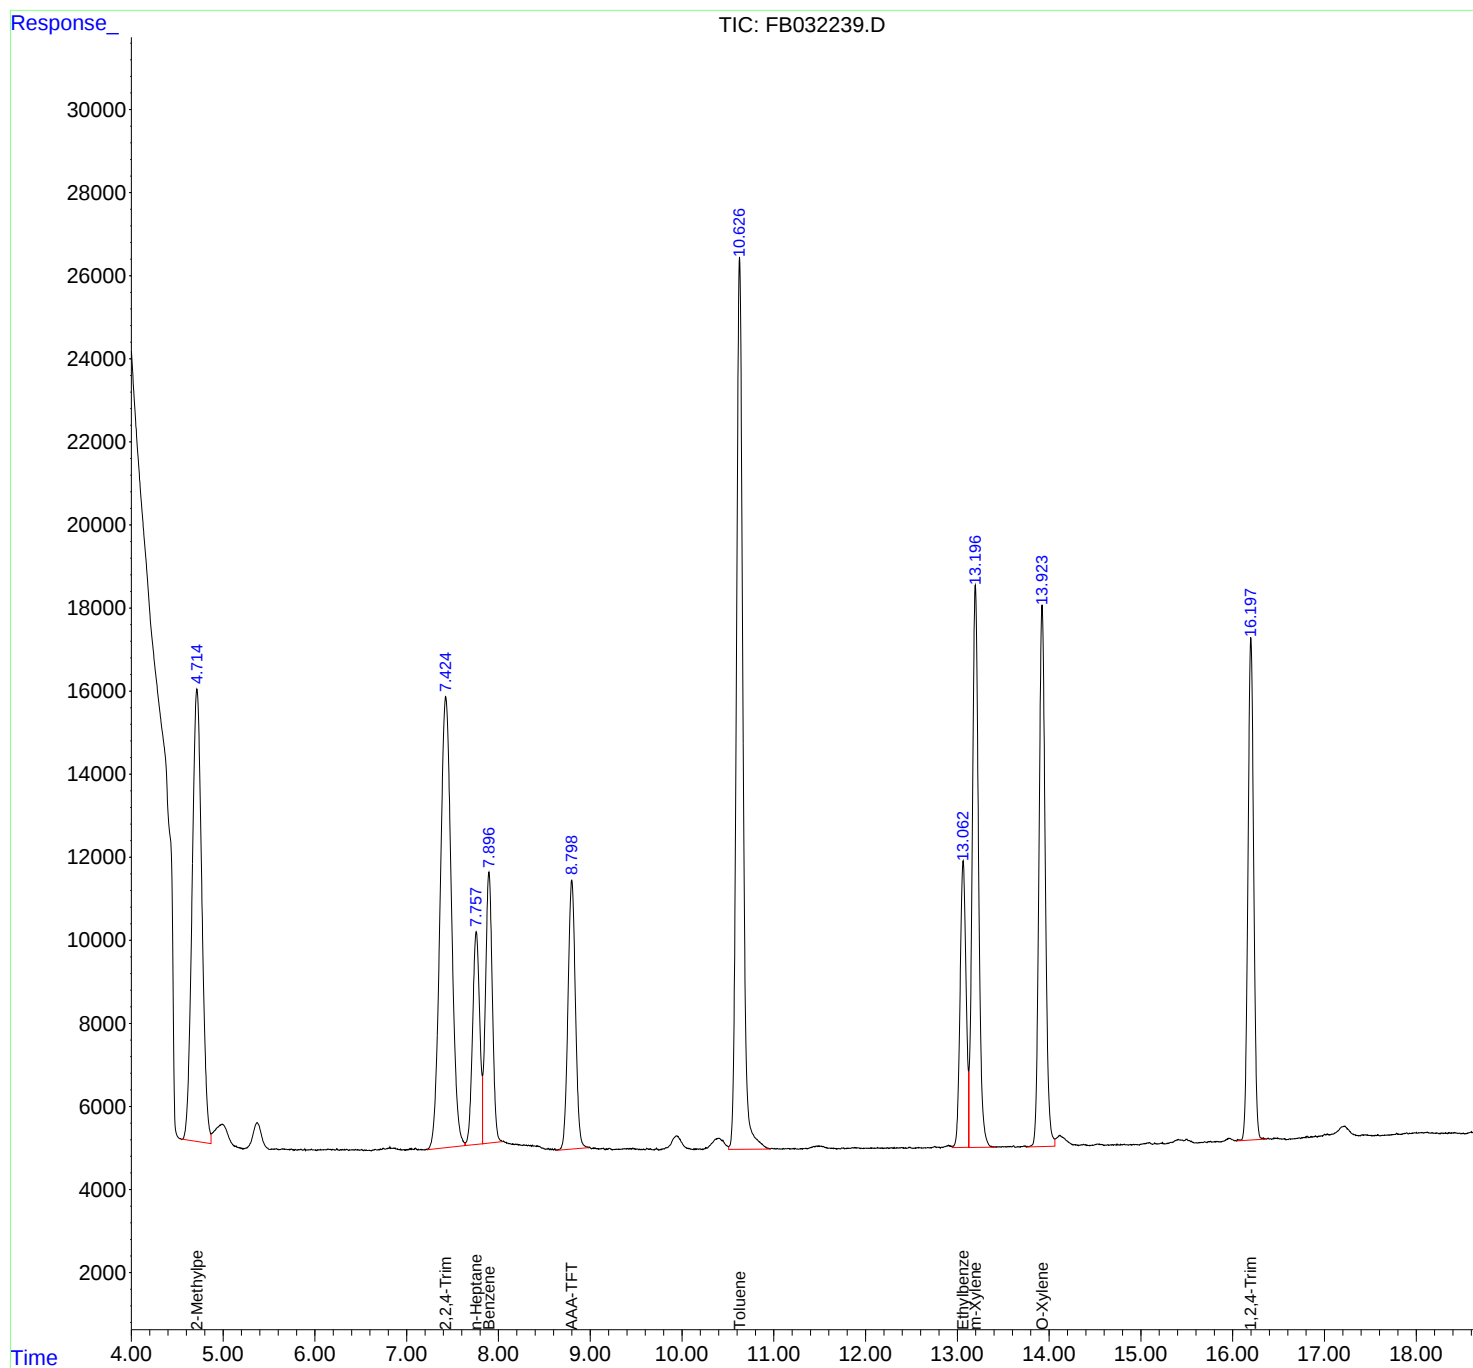


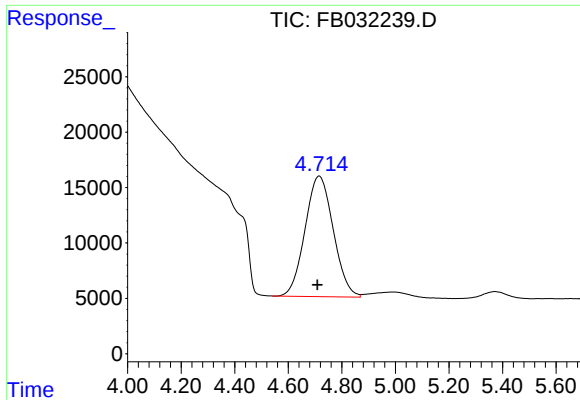

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: 0.007 min
Response: 797639
Conc: 29.54 ng/ml

Instrument :
FID_E
ClientSampleId :

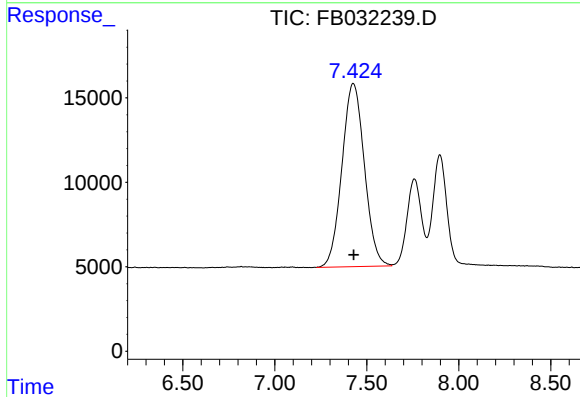


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.004 min
Response: 920023
Conc: 32.57 ng/ml

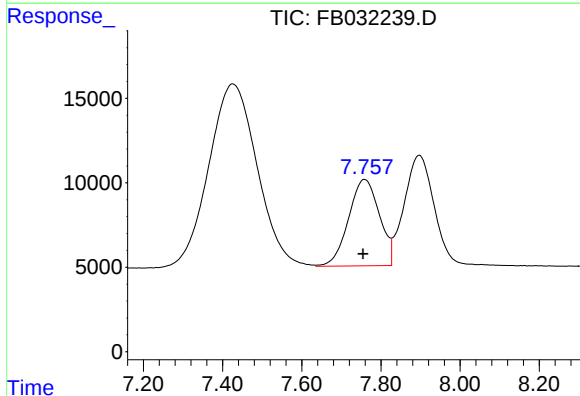


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 277011
Conc: 10.14 ng/ml

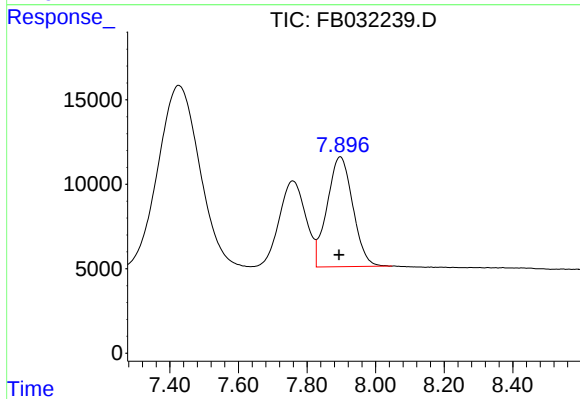

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.004 min
Response: 338968
Conc: 9.38 ng/ml

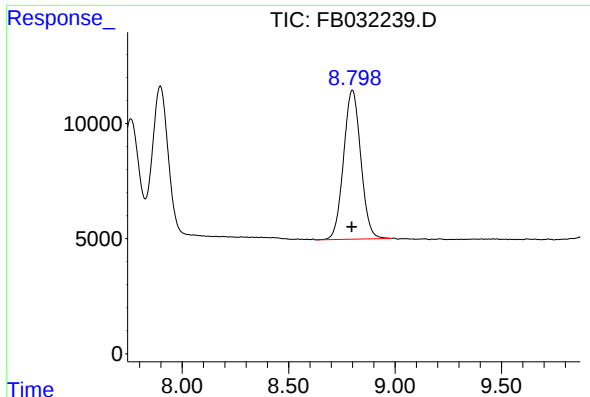

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.004 min
Response: 364181
Conc: 20.35 ng/ml

Instrument :
FID_E
ClientSampleId :

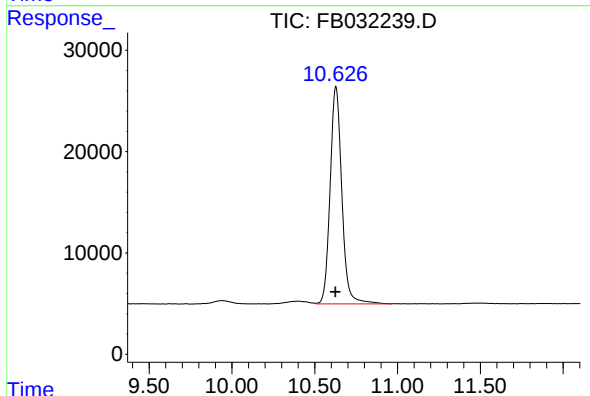


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.002 min
Response: 1054461
Conc: 28.31 ng/ml

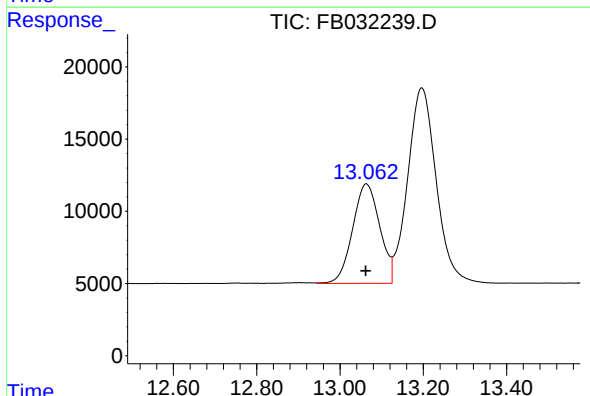


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.002 min
Response: 311205
Conc: 9.52 ng/ml

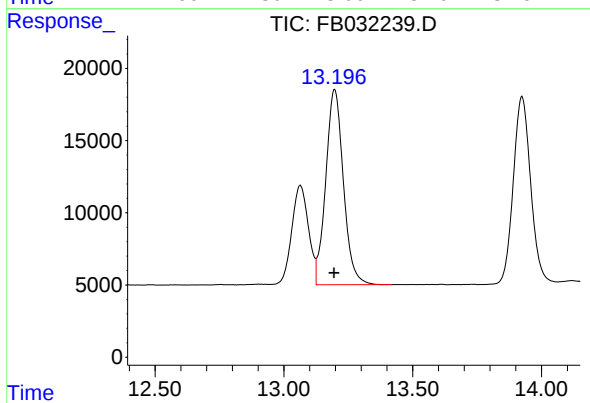

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 643824
Conc: 18.89 ng/ml

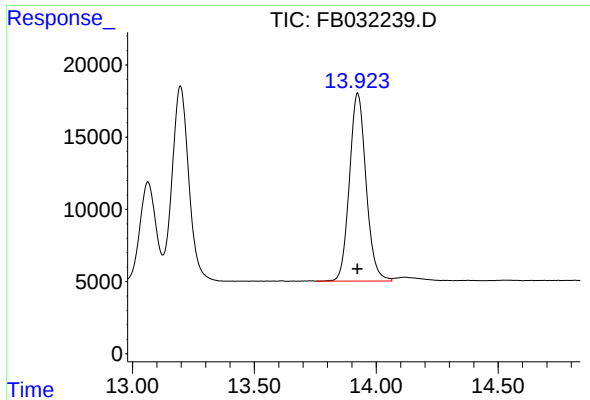

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.001 min
Response: 616388
Conc: 18.88 ng/ml

Instrument :
FID_E
ClientSampleId :

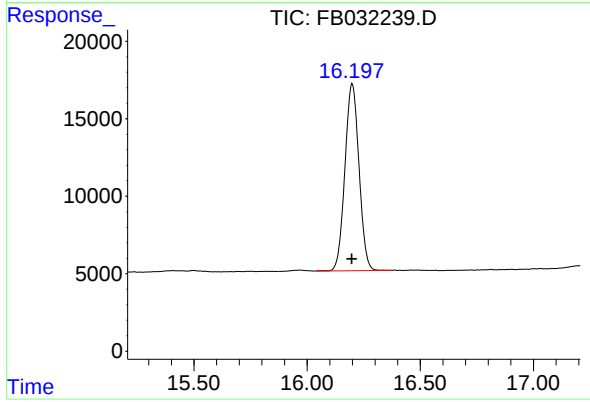

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.002 min
Response: 522635
Conc: 18.68 ng/ml