

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100825\
 Data File : FB032240.D
 Signal(s) : FID2B.CH
 Acq On : 8 Oct 2025 11:34
 Operator : YP/AJ
 Sample : BSF1008S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Oct 09 04:10:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
 Quant Title :
 QLast Update : Mon Sep 22 12:16:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	383084	21.402 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	863985	31.992 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	982543	34.782 ng/ml
3) t n-Heptane	7.759	314183	11.499 ng/ml
4) t Benzene	7.897	374220	10.355 ng/ml
6) t Toluene	10.628	1120985	30.098 ng/ml
7) t Ethylbenzene	13.064	331461	10.140 ng/ml
8) t m-Xylene	13.197	688894	20.211 ng/ml
9) t O-Xylene	13.924	663907	20.331 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	571773	20.441 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB100825\
Data File : FB032240.D
Signal(s) : FID2B.CH
Acq On : 8 Oct 2025 11:34
Operator : YP/AJ
Sample : BSF1008S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Oct 09 04:10:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB092225.M
Quant Title :
QLast Update : Mon Sep 22 12:16:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

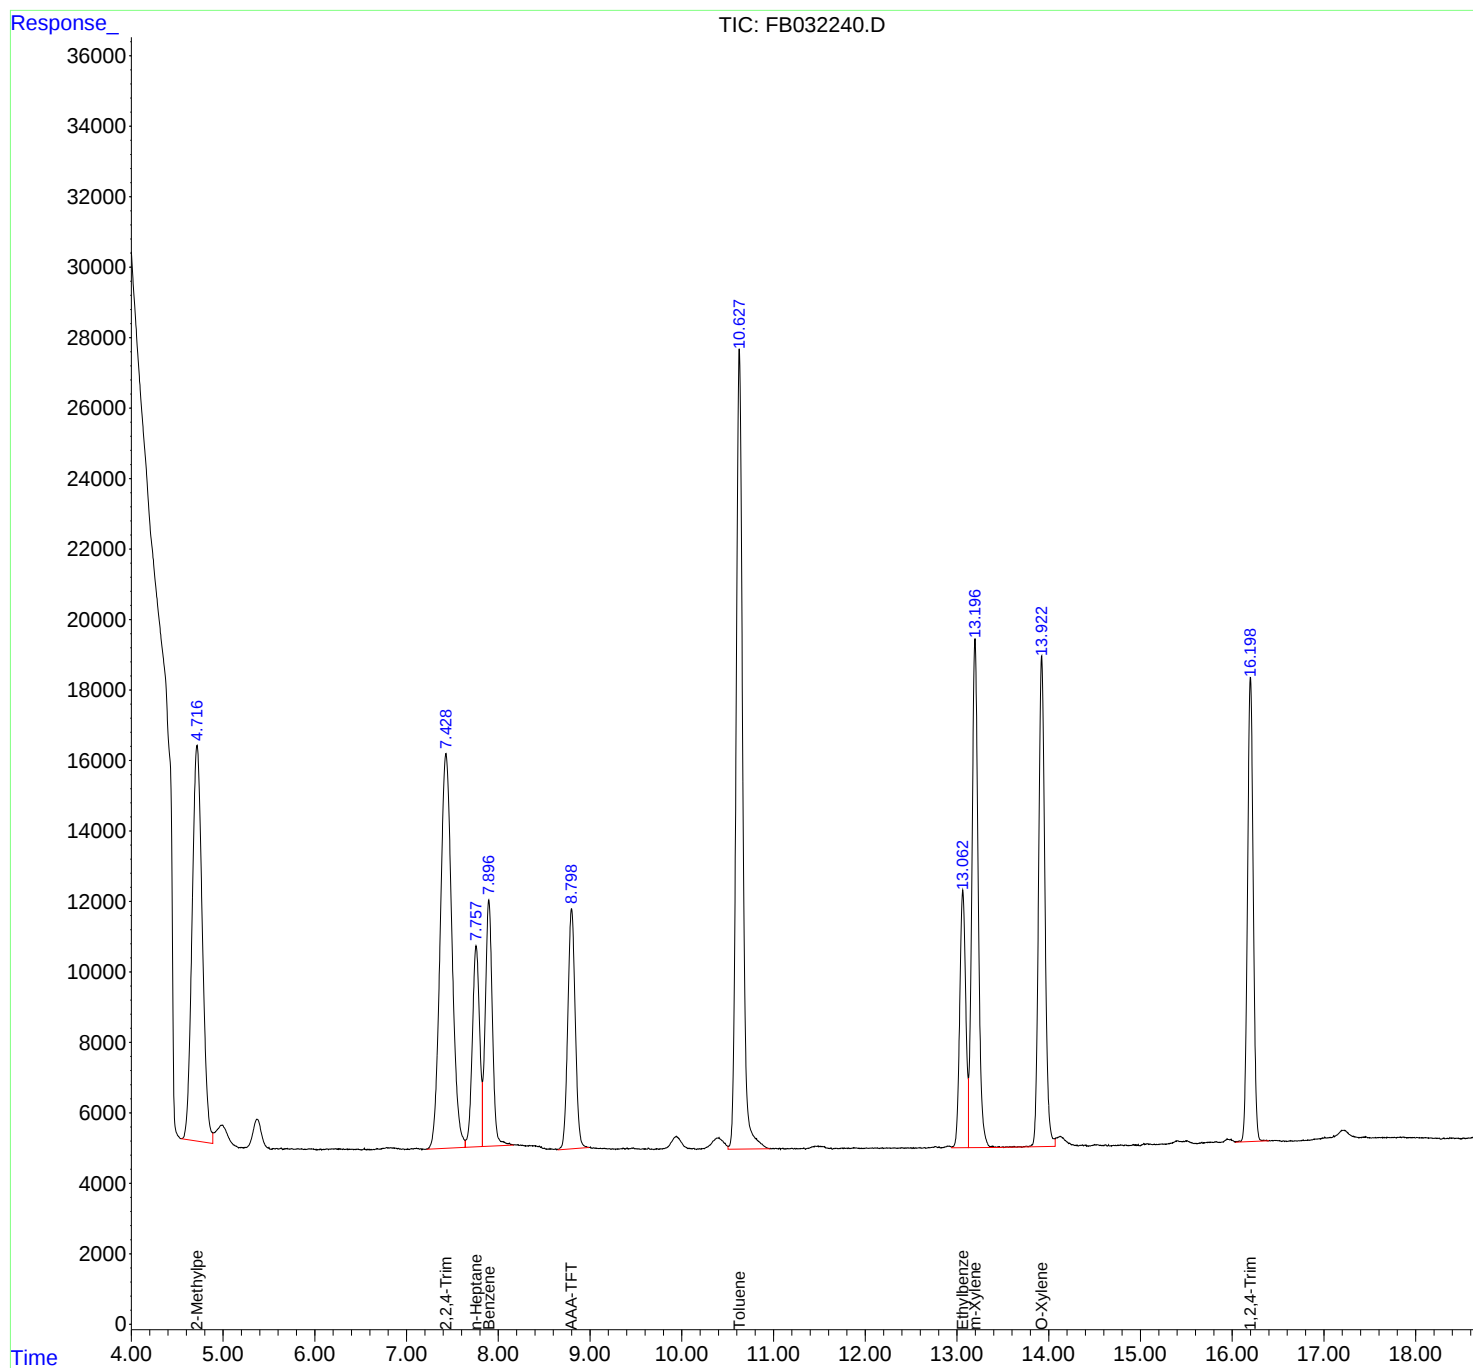


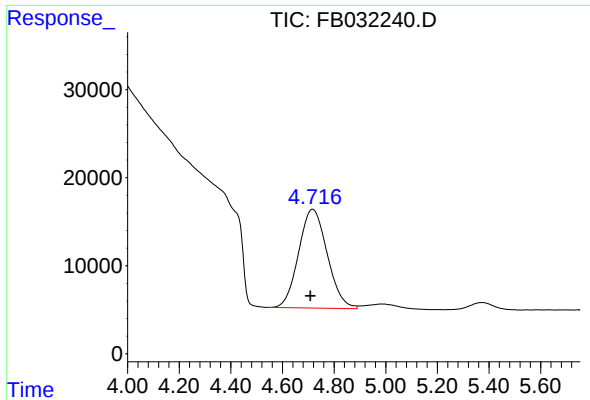

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.008 min
Response: 863985
Conc: 31.99 ng/ml

Instrument :
FID_E
ClientSampleId :

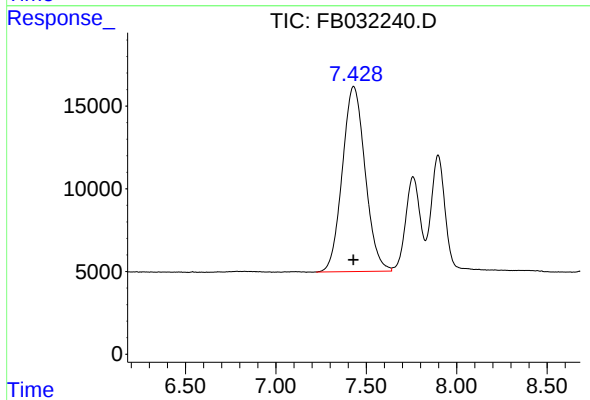


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.000 min
Response: 982543
Conc: 34.78 ng/ml

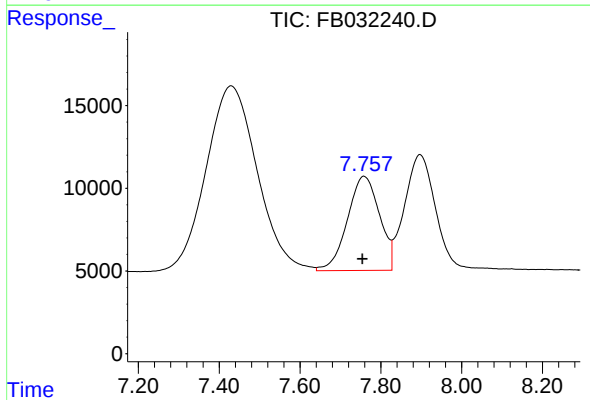


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 314183
Conc: 11.50 ng/ml

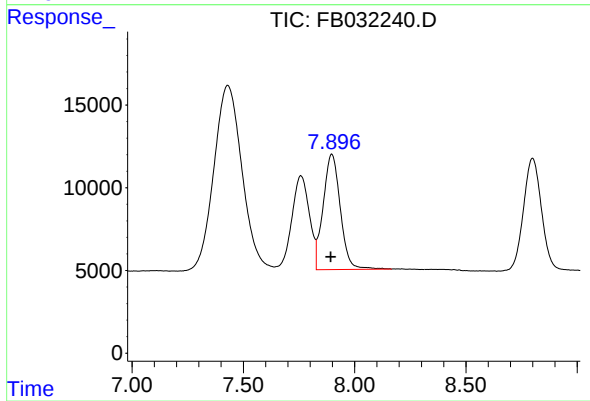

#4 Benzene


R.T.: 7.897 min
Delta R.T.: 0.004 min
Response: 374220
Conc: 10.35 ng/ml

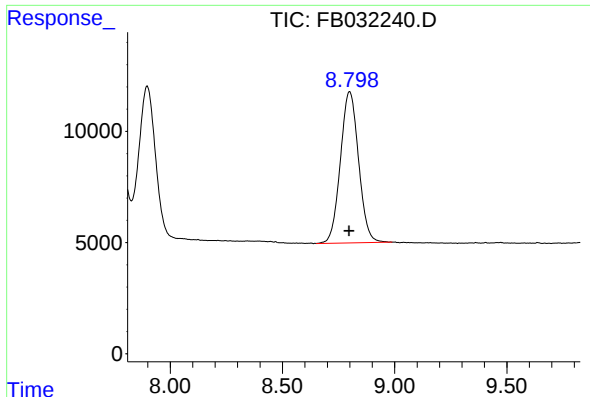

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 383084
Conc: 21.40 ng/ml

Instrument :
FID_E
ClientSampleId :

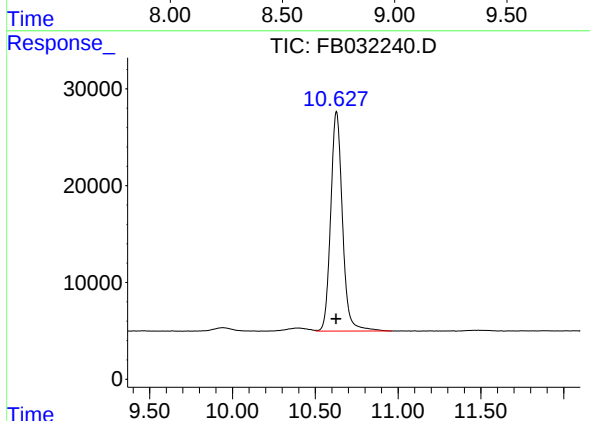


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.003 min
Response: 1120985
Conc: 30.10 ng/ml

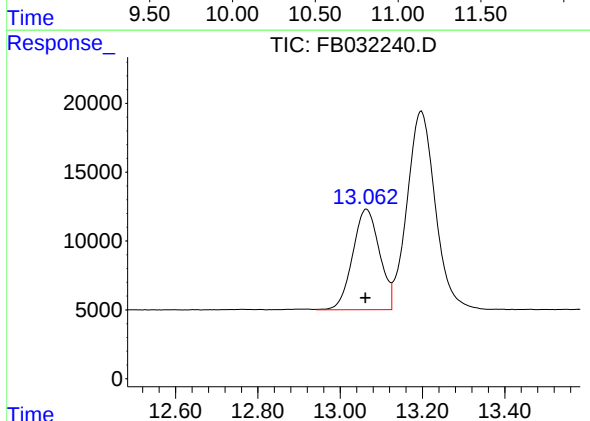


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.002 min
Response: 331461
Conc: 10.14 ng/ml

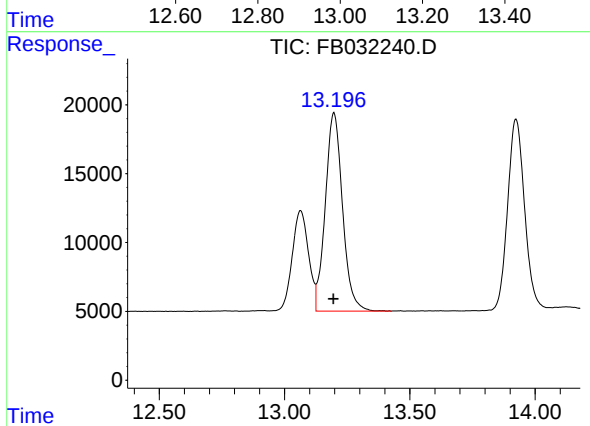

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.002 min
Response: 688894
Conc: 20.21 ng/ml

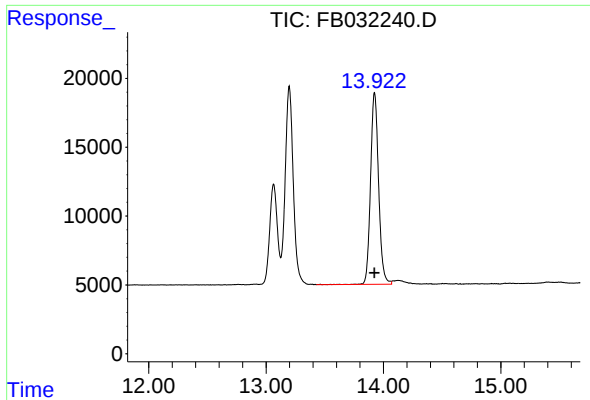

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.001 min
Response: 663907
Conc: 20.33 ng/ml

Instrument :
FID_E
ClientSampleId :

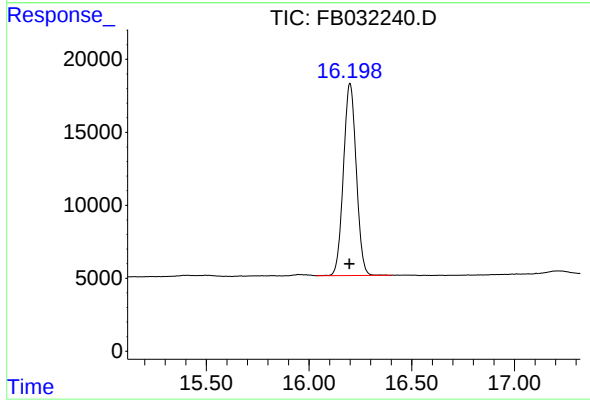

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.002 min
Response: 571773
Conc: 20.44 ng/ml