

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100825\  
Data File : FB032242.D  
Signal(s) : FID2B.CH  
Acq On : 8 Oct 2025 12:47  
Operator : YP/AJ  
Sample : Q3305-01  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 09 04:10:51 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB092225.M  
Quant Title :  
QLast Update : Mon Sep 22 12:16:10 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.804  | 1683982  | 94.080 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.638 | 619271   | 16.627 ng/ml |
| 7) t Ethylbenzene            | 13.061 | 126773   | 3.878 ng/ml  |
| 8) t m-Xylene                | 13.169 | 392830   | 11.525 ng/ml |
| 10) t 1,2,4-Trimethylbenzene | 16.203 | 115351   | 4.124 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB100825\  
Data File : FB032242.D  
Signal(s) : FID2B.CH  
Acq On : 8 Oct 2025 12:47  
Operator : YP/AJ  
Sample : Q3305-01  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Oct 09 04:10:51 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB092225.M  
Quant Title :  
QLast Update : Mon Sep 22 12:16:10 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

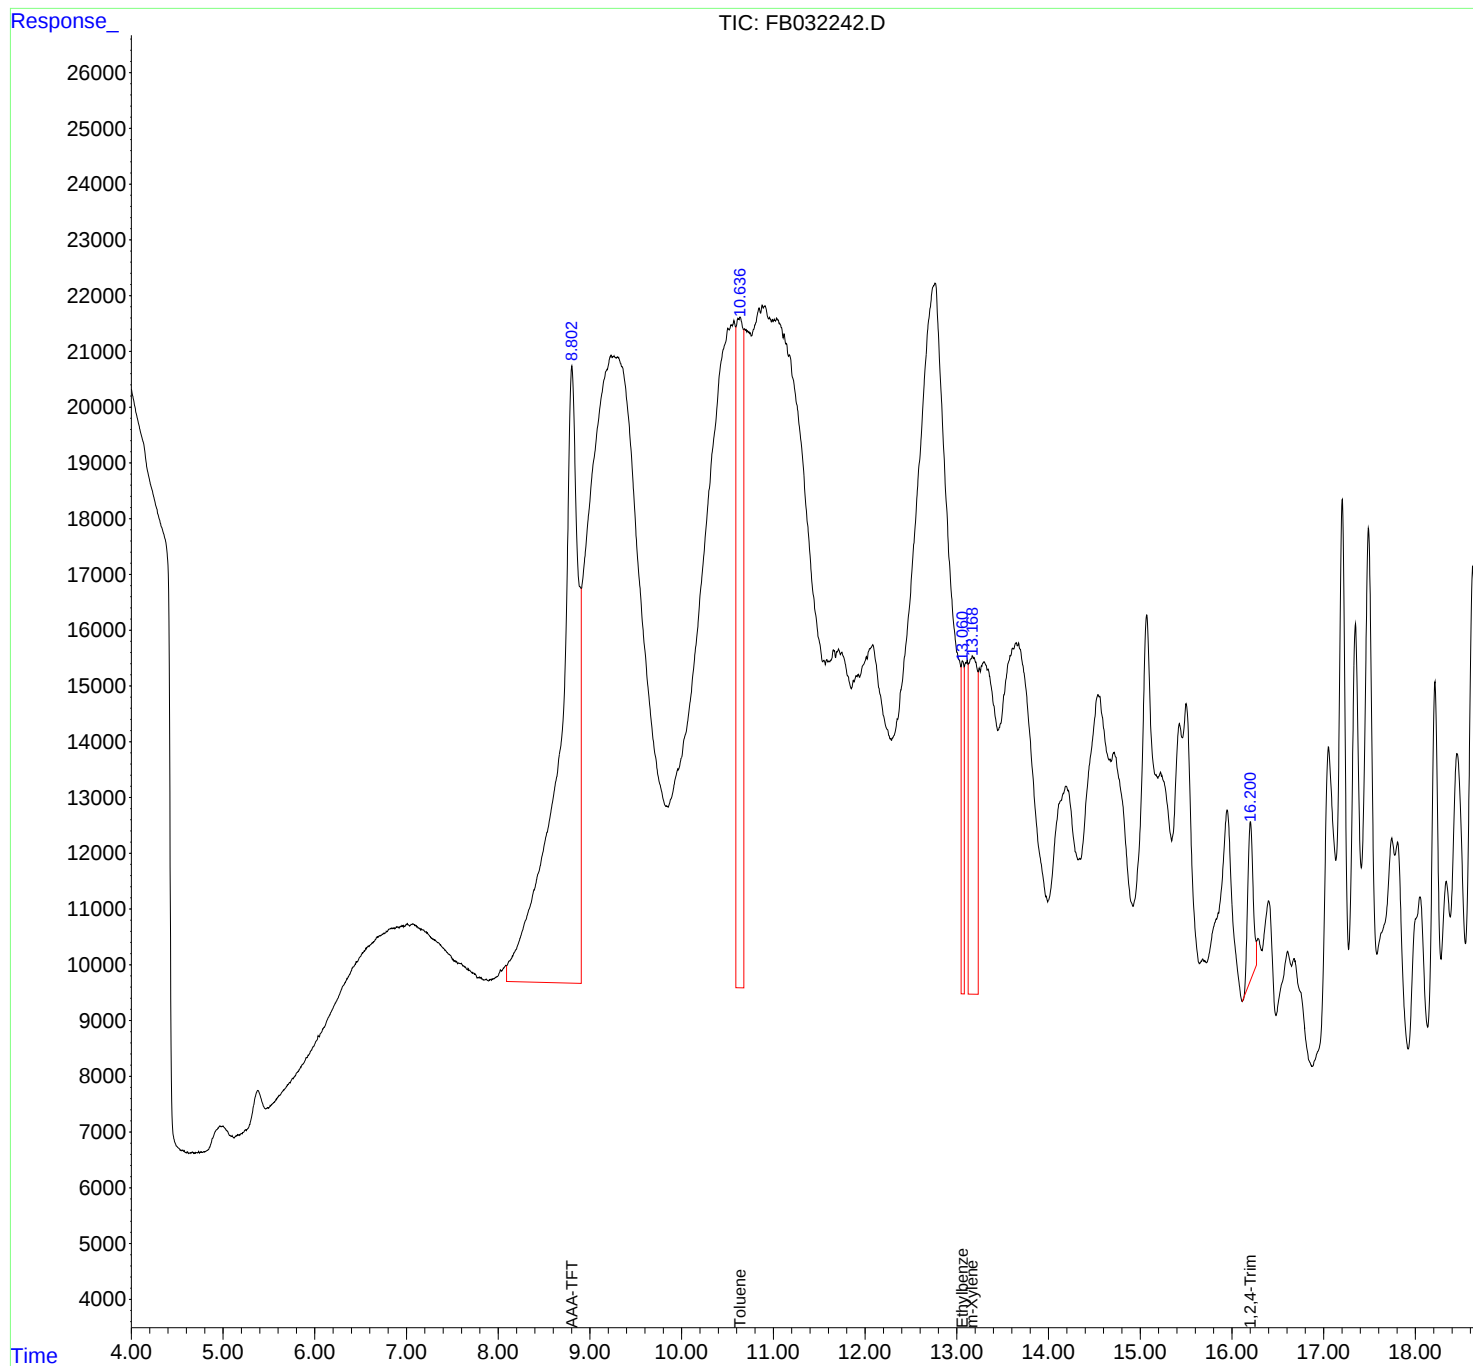


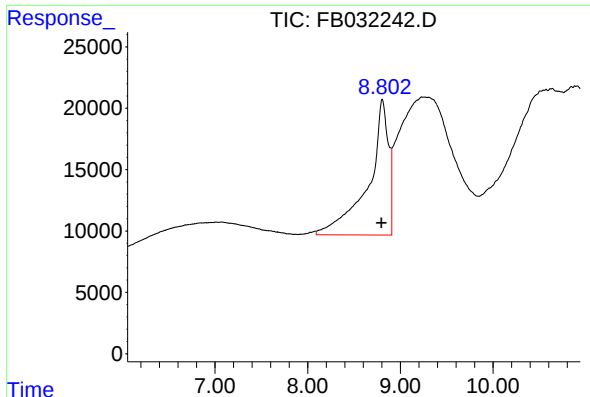

#5 AAA-TFT


R.T.: 8.804 min  
Delta R.T.: 0.008 min  
Response: 1683982  
Conc: 94.08 ng/ml

Instrument :  
FID\_E  
ClientSampleId :

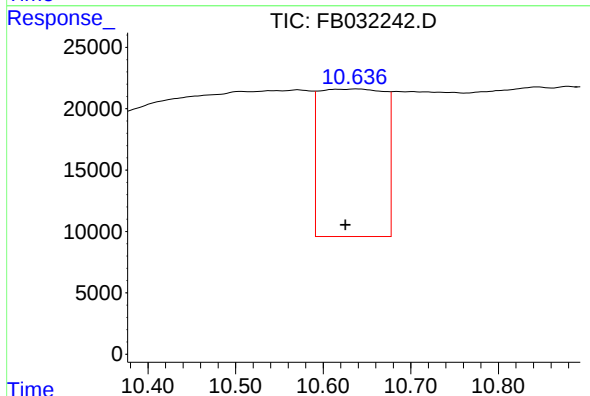


#6 Toluene

R.T.: 10.638 min  
Delta R.T.: 0.012 min  
Response: 619271  
Conc: 16.63 ng/ml

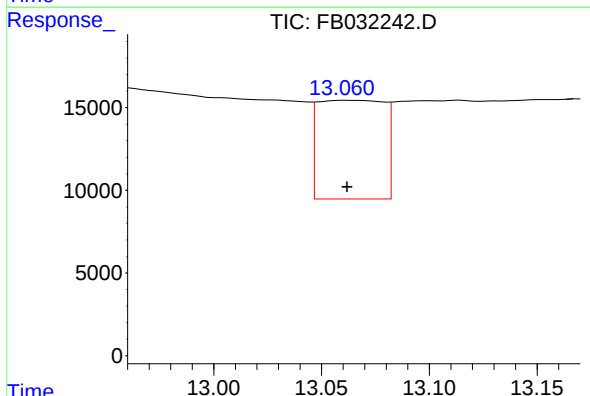


#7 Ethylbenzene

R.T.: 13.061 min  
Delta R.T.: 0.000 min  
Response: 126773  
Conc: 3.88 ng/ml

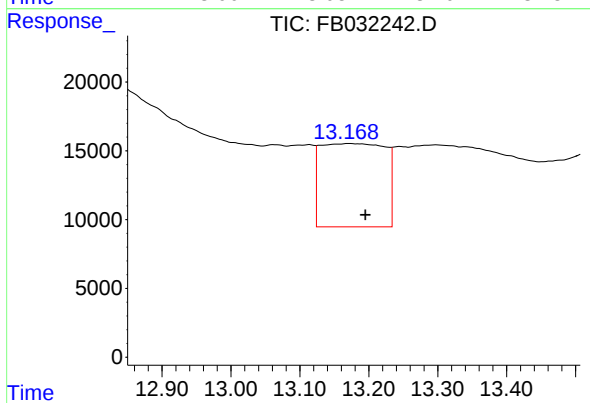

#8 m-Xylene

R.T.: 13.169 min  
Delta R.T.: -0.026 min  
Response: 392830  
Conc: 11.53 ng/ml

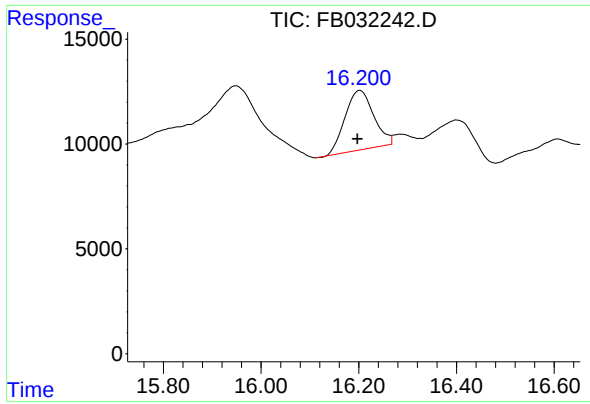

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min

Delta R.T.: 0.005 min

Response: 115351

Conc: 4.12 ng/ml

Instrument :

FID\_E

ClientSampleId :