

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100923\
Data File : FE044722.D
Signal(s) : FID1B.ch
Acq On : 09 Oct 2023 10:43
Operator : YP\AJ
Sample : PB156110BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB156110BL

Integration File: autoint1.e
Quant Time: Oct 09 23:43:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.014	3498255	23.844 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100923\
Data File : FE044722.D
Signal(s) : FID1B.ch
Acq On : 09 Oct 2023 10:43
Operator : YP\AJ
Sample : PB156110BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB156110BL

Integration File: autoint1.e
Quant Time: Oct 09 23:43:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

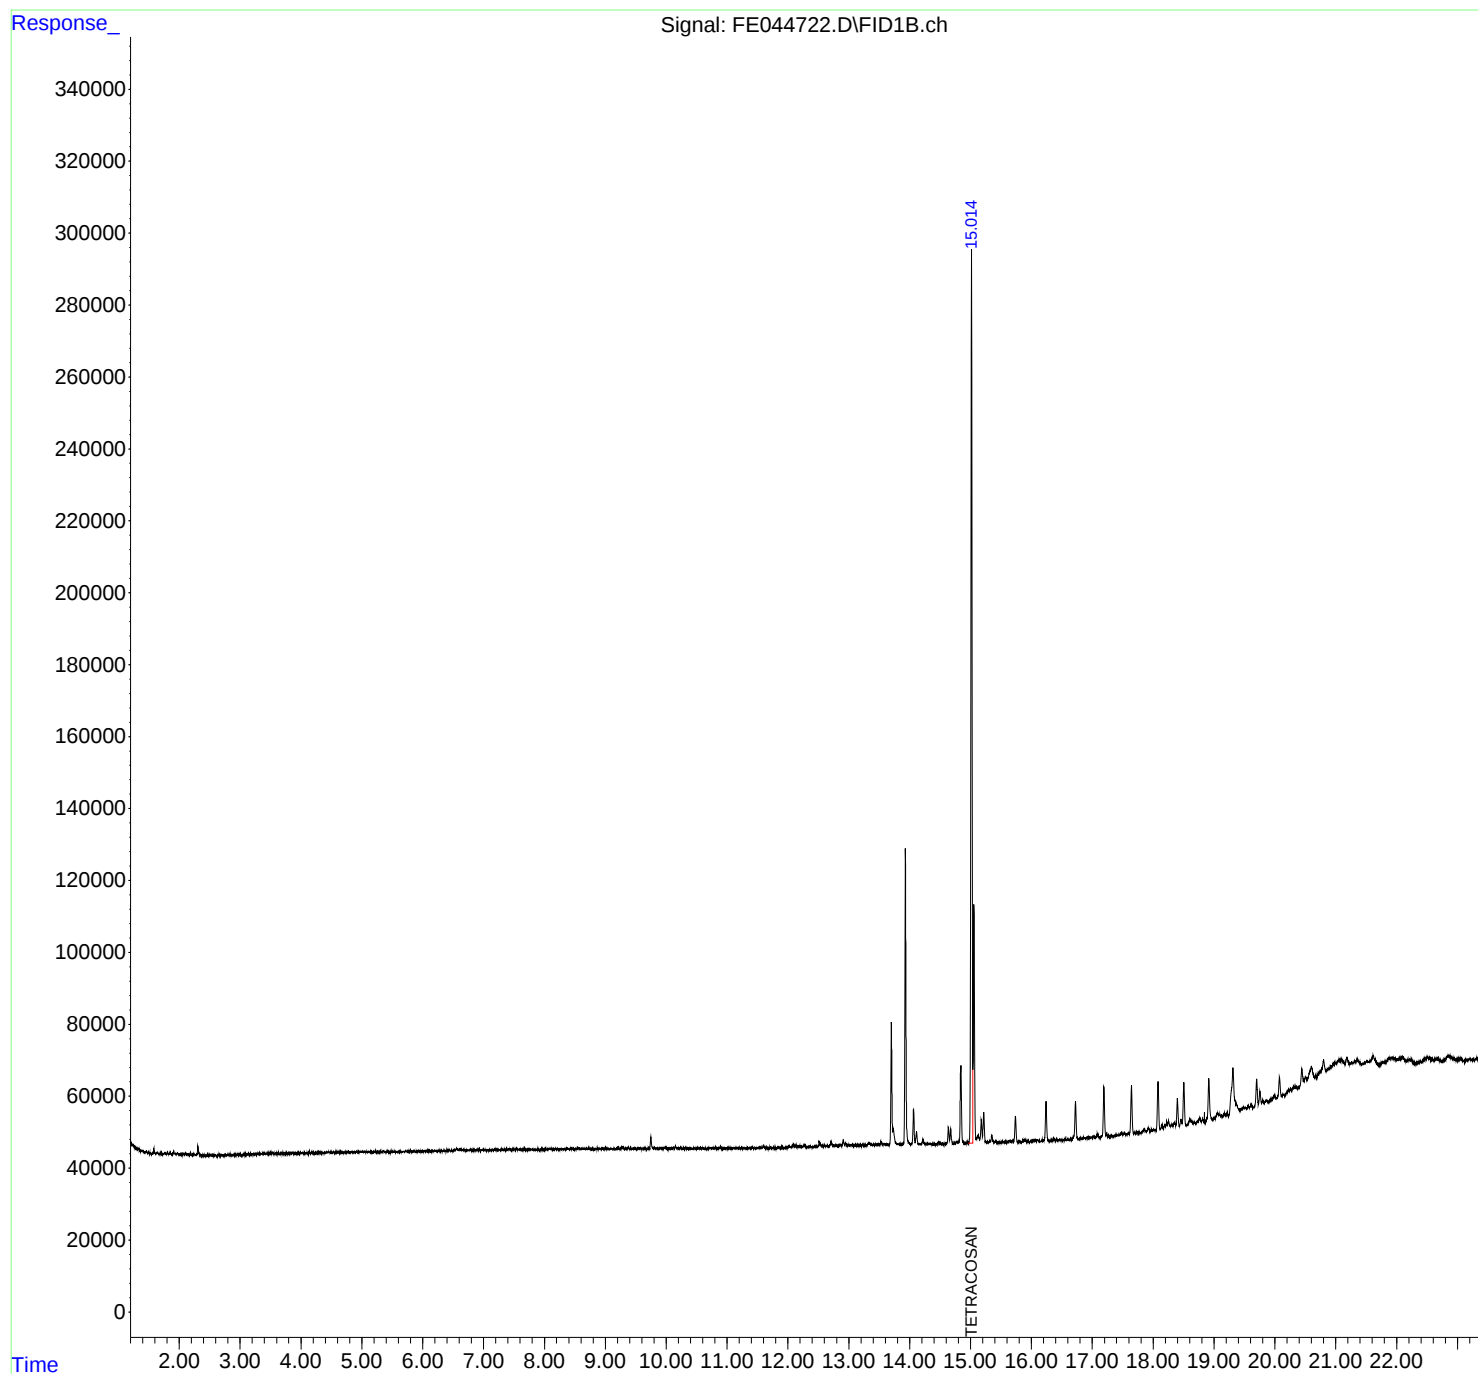

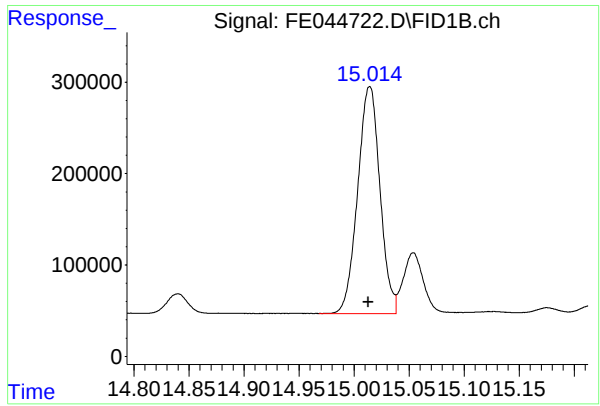

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.014 min
Delta R.T.: 0.001 min
Response: 3498255
Conc: 23.84 ug/ml

Instrument :
FID_E
ClientSampleId :
PB156110BL