

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100923\
Data File : FE044726.D
Signal(s) : FID1B.ch
Acq On : 09 Oct 2023 12:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 09 23:44:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.012	2451980	16.713 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE100923\
Data File : FE044726.D
Signal(s) : FID1B.ch
Acq On : 09 Oct 2023 12:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 09 23:44:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100323.M
Quant Title :
QLast Update : Tue Oct 03 12:58:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

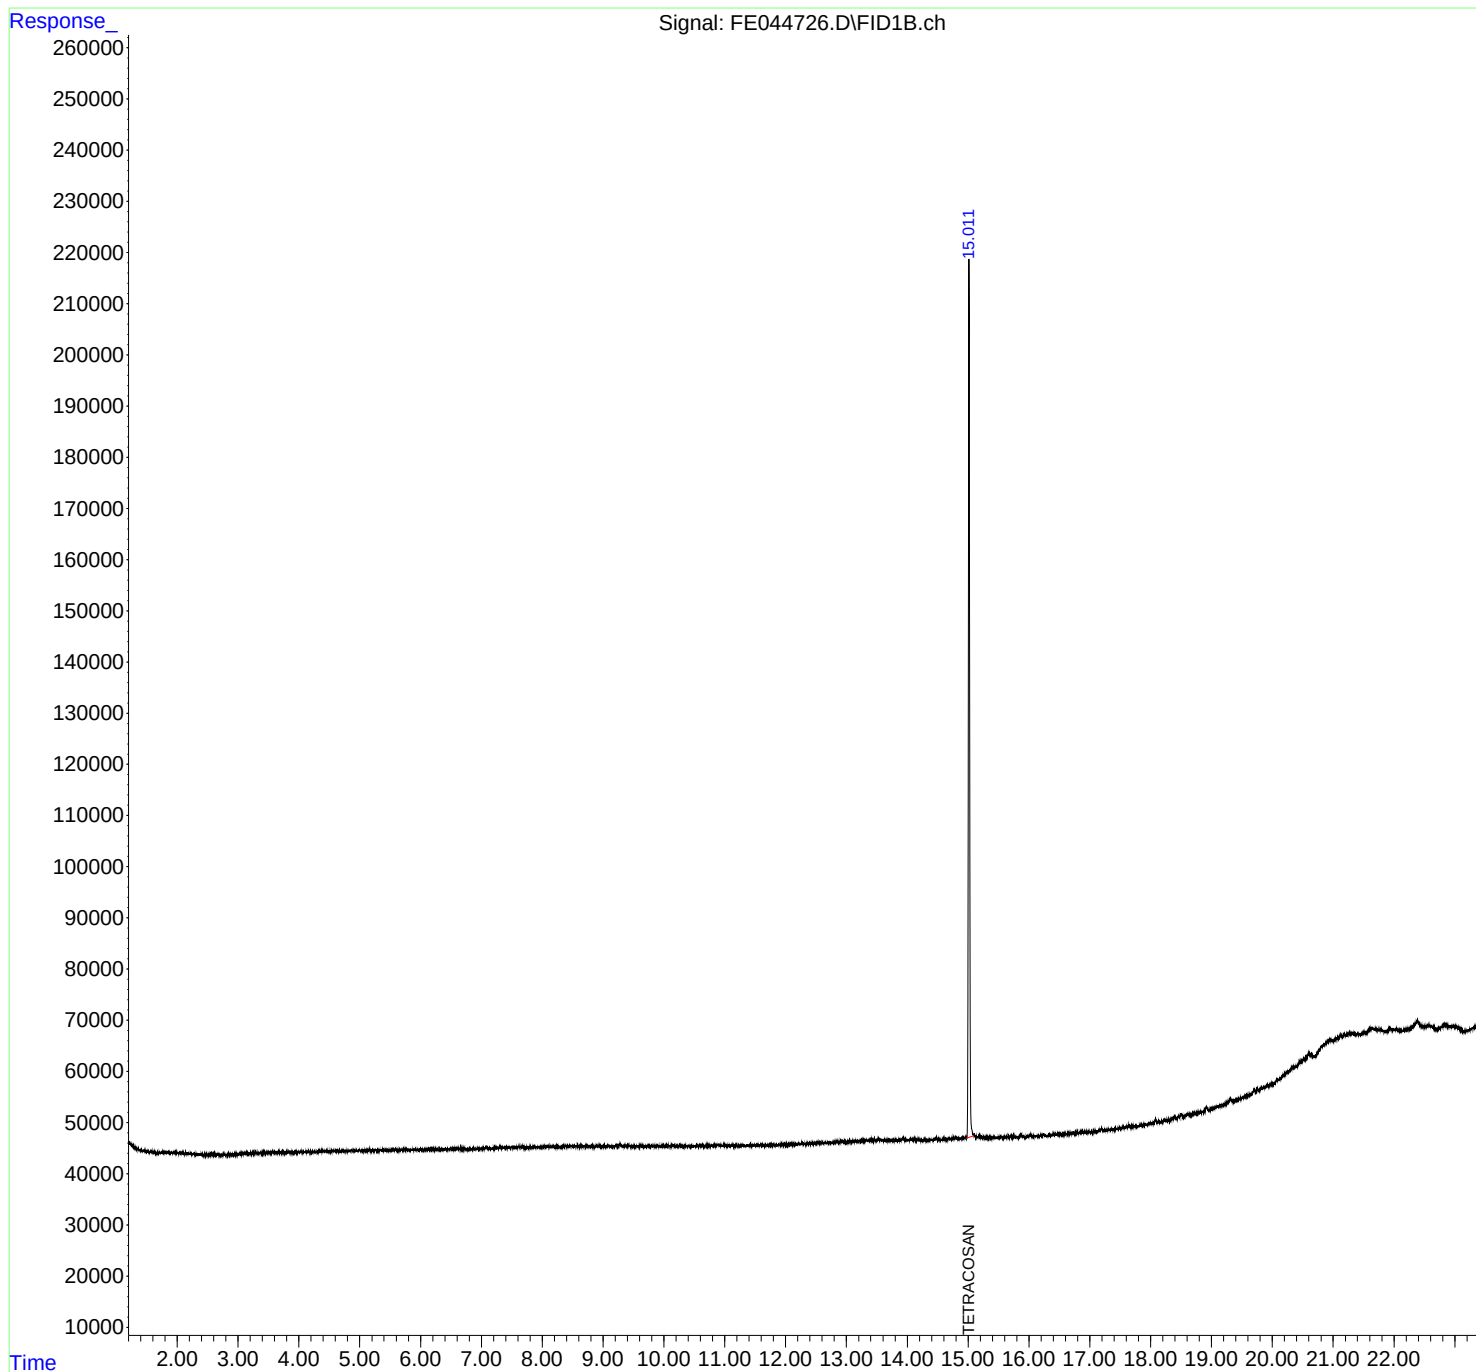

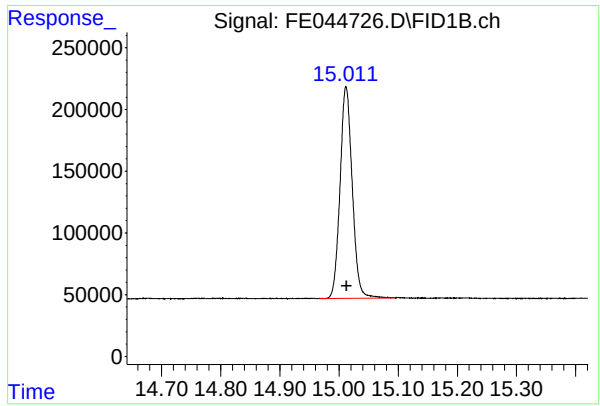

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.012 min

Delta R.T.: -0.001 min

Response: 2451980

Conc: 16.71 ug/ml

Instrument :

FID_E

ClientSampleId :

I.BLK