

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100925AL\  
 Data File : FE056285.D  
 Signal(s) : FID1B.ch  
 Acq On : 09 Oct 2025 21:56  
 Operator : YP\AJ  
 Sample : Q3313-01D  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 ETGI-360

Integration File: autoint1.e  
 Quant Time: Oct 10 01:54:08 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 092425.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Sep 24 12:55:37 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 12.061 | 4603233    | 24.531 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 49.06%       |
| 12) S 1-chlorooctadecane (S... | 13.498 | 3699050    | 26.504 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 53.01%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE100925AL\  
Data File : FE056285.D  
Signal(s) : FID1B.ch  
Acq On : 09 Oct 2025 21:56  
Operator : YP\AJ  
Sample : Q3313-01D  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
ETGI-360

Integration File: autoint1.e  
Quant Time: Oct 10 01:54:08 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 092425.M  
Quant Title : GC Extractables  
QLast Update : Wed Sep 24 12:55:37 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 u1  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

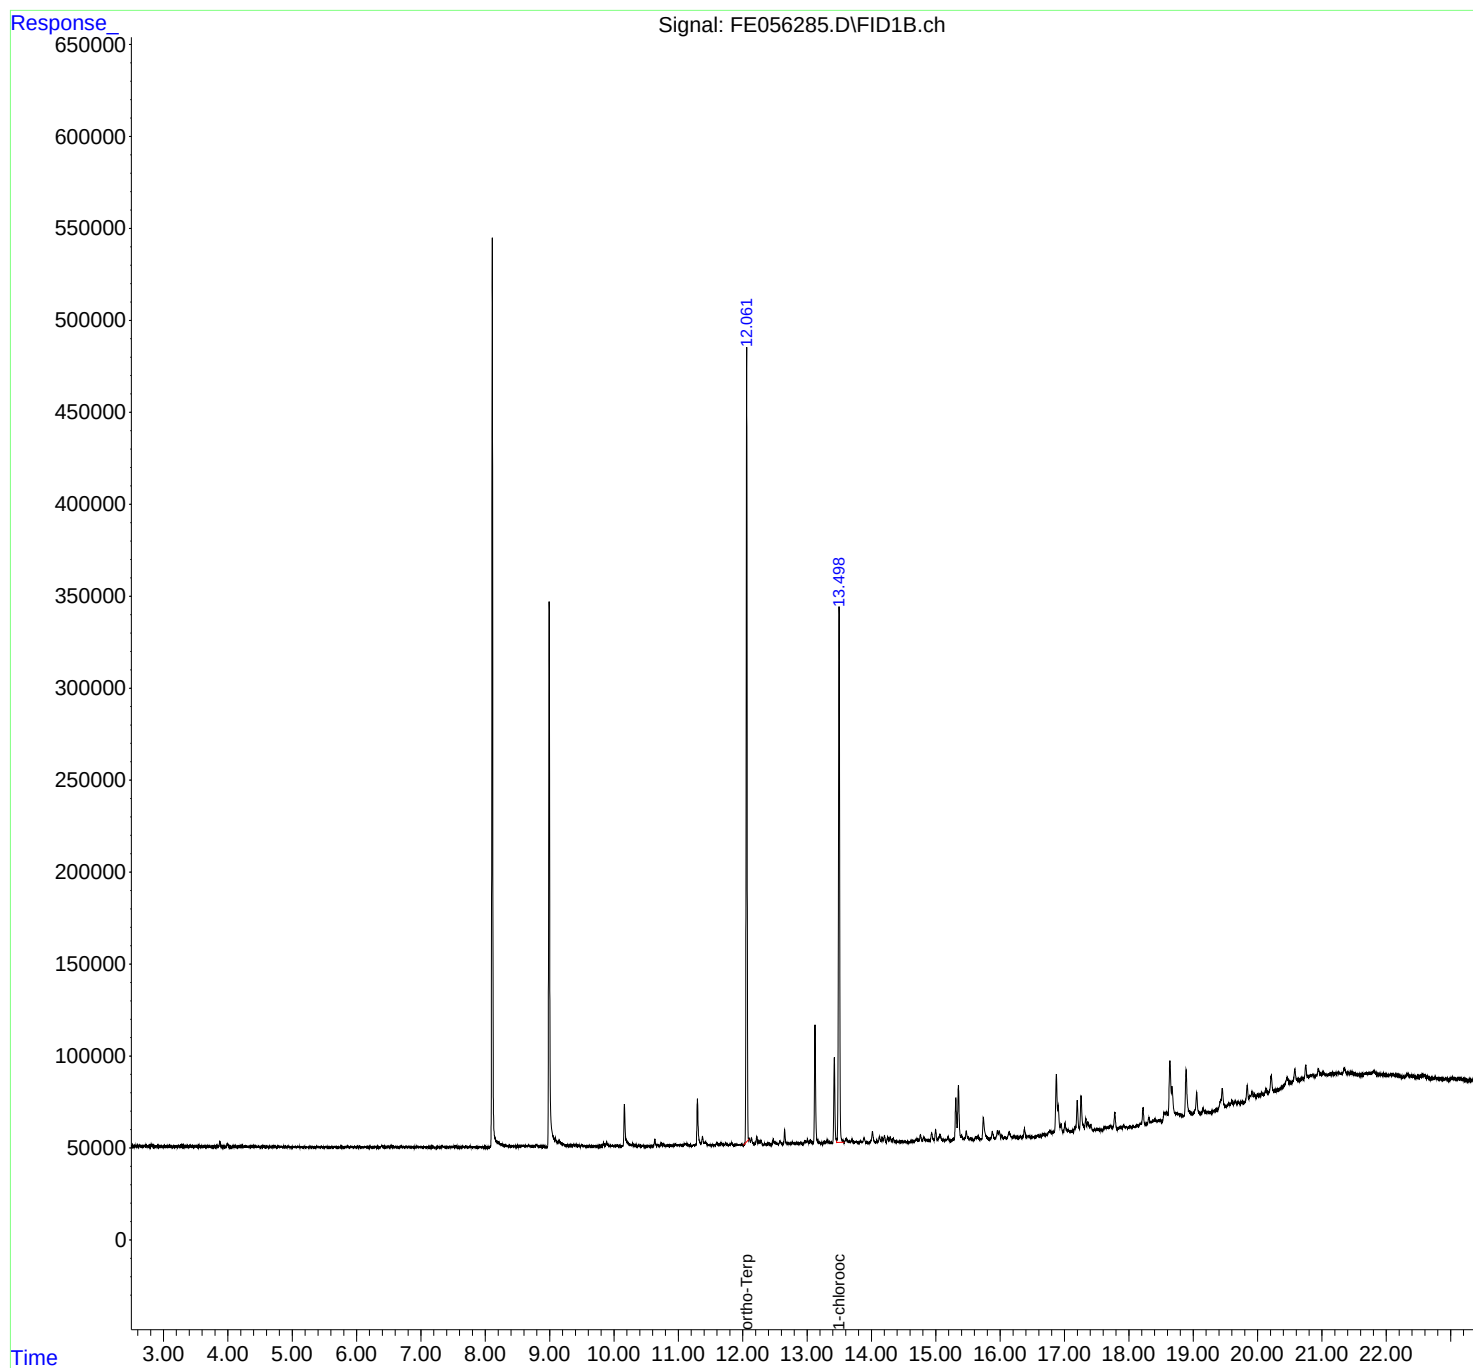


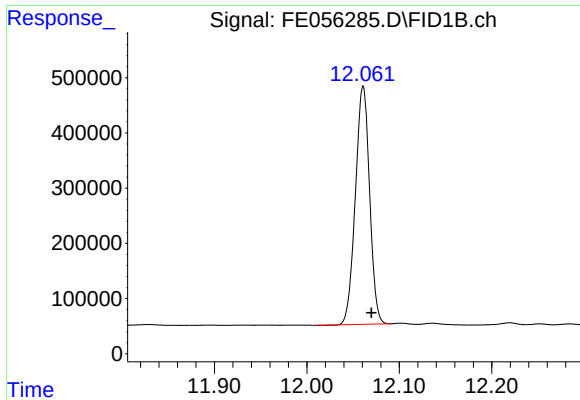

#9 ortho-Terphenyl (SURR)

R.T.: 12.061 min  
Delta R.T.: -0.009 min  
Response: 4603233  
Conc: 24.53 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
ETGI-360

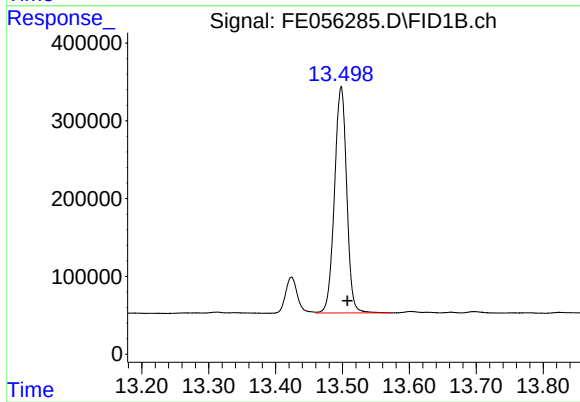

#12 1-chlorooctadecane (SURR)

R.T.: 13.498 min  
Delta R.T.: -0.010 min  
Response: 3699050  
Conc: 26.50 ug/ml