

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101025\
Data File : FF016555.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2025 11:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 10 23:45:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100225.M
Quant Title :
QLast Update : Fri Oct 03 03:40:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.068	1855254	15.774 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.559f	61760	0.751 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101025\
Data File : FF016555.D
Signal(s) : FID2B.ch
Acq On : 10 Oct 2025 11:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 10 23:45:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100225.M
Quant Title :
QLast Update : Fri Oct 03 03:40:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

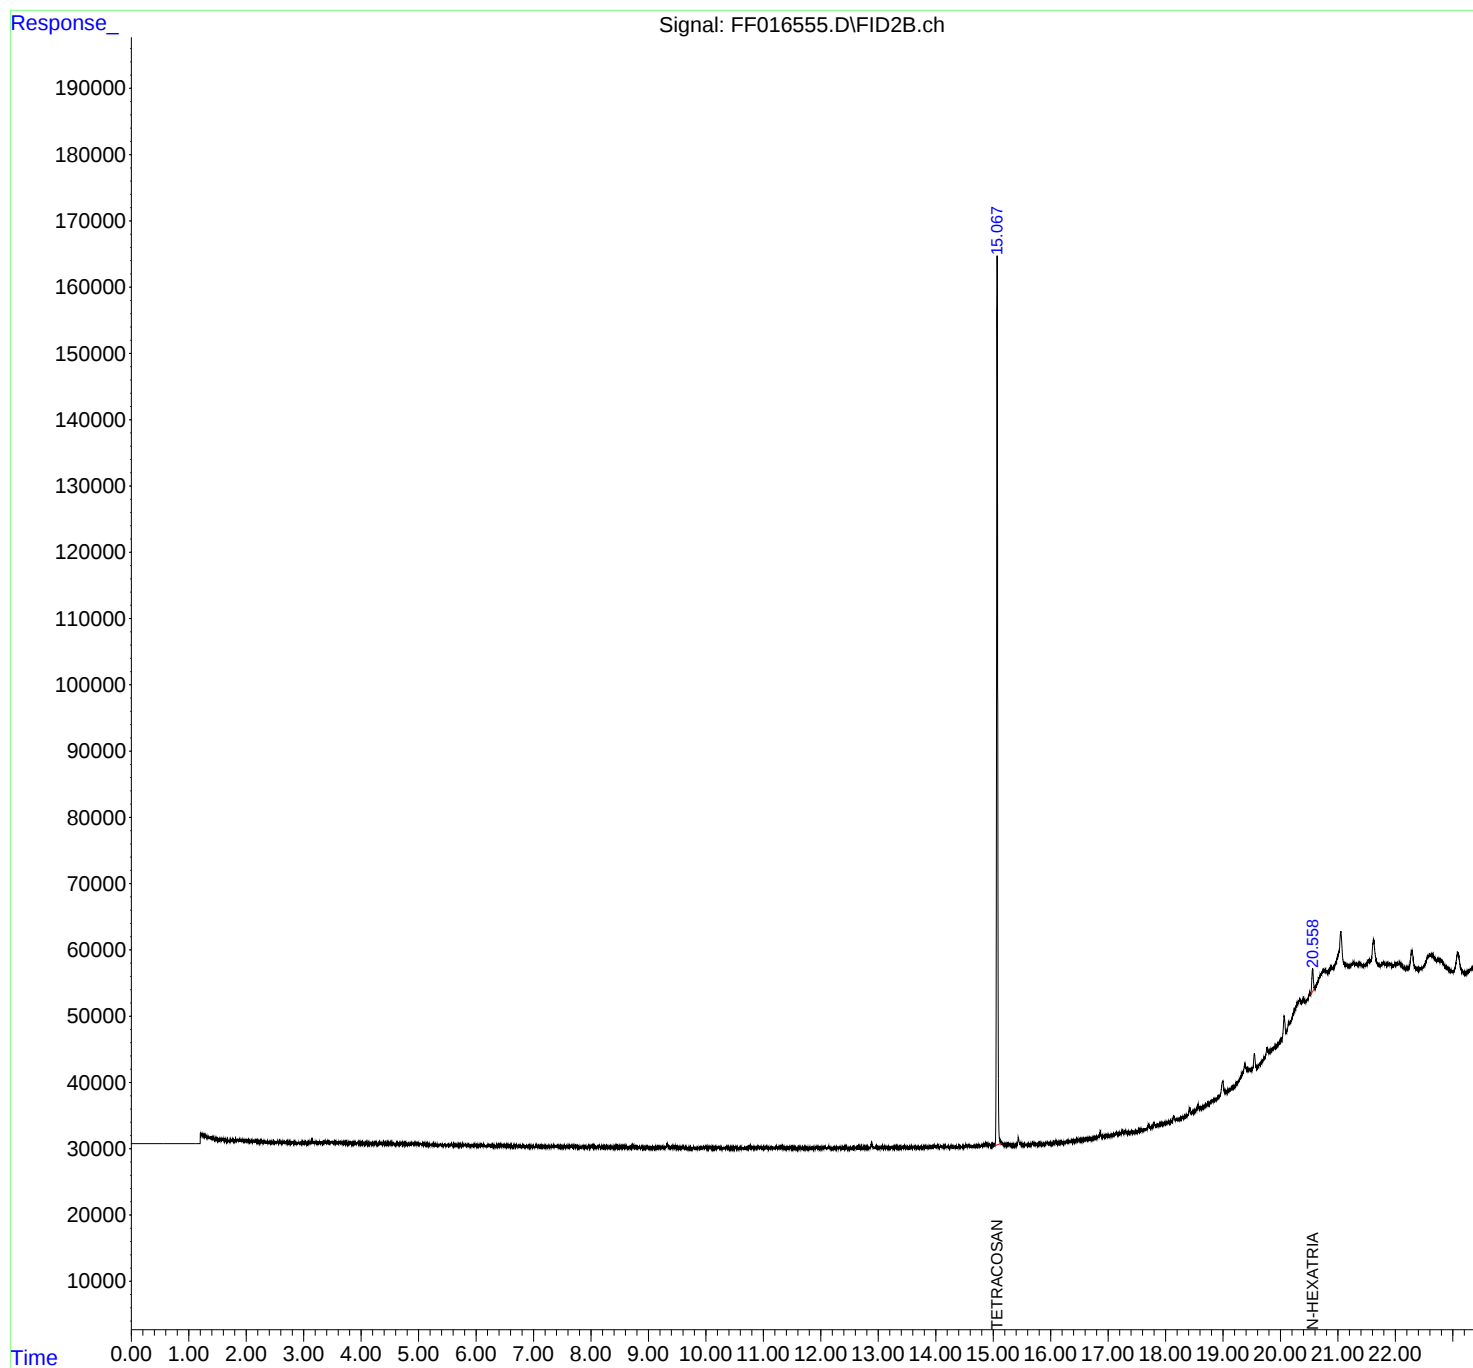


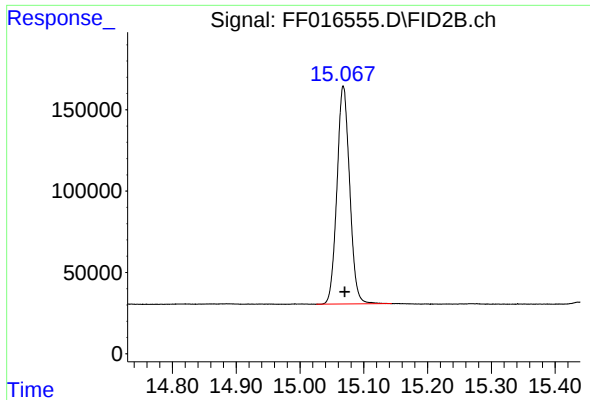

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.068 min
Delta R.T.: -0.002 min
Response: 1855254
Conc: 15.77 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK

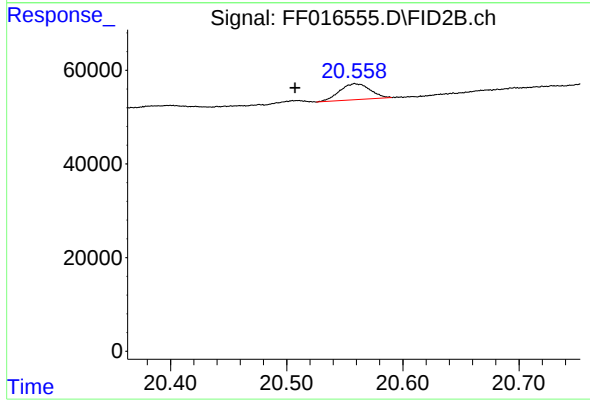

#16 N-HEXATRIACONTANE

R.T.: 20.559 min
Delta R.T.: 0.052 min
Response: 61760
Conc: 0.75 ug/ml