

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101118\
Data File : FE028897.D
Signal(s) : FID1B.CH
Acq On : 11 Oct 2018 7:46
Operator : DD\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 11 14:41:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092118.M
Quant Title :
QLast Update : Fri Sep 21 07:24:23 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	15.124	675434	3.873 ug/ml
12)	N-DOTRIACONTANE	18.852	1626766	12.522 ug/ml
14)	N-HEXATRIACONTANE	20.405	1442495	14.275 ug/ml
15)	N-TETRACONTANE	22.205	876381	12.120 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101118\
Data File : FE028897.D
Signal(s) : FID1B.CH
Acq On : 11 Oct 2018 7:46
Operator : DD\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 11 14:41:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE092118.M
Quant Title :
QLast Update : Fri Sep 21 07:24:23 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

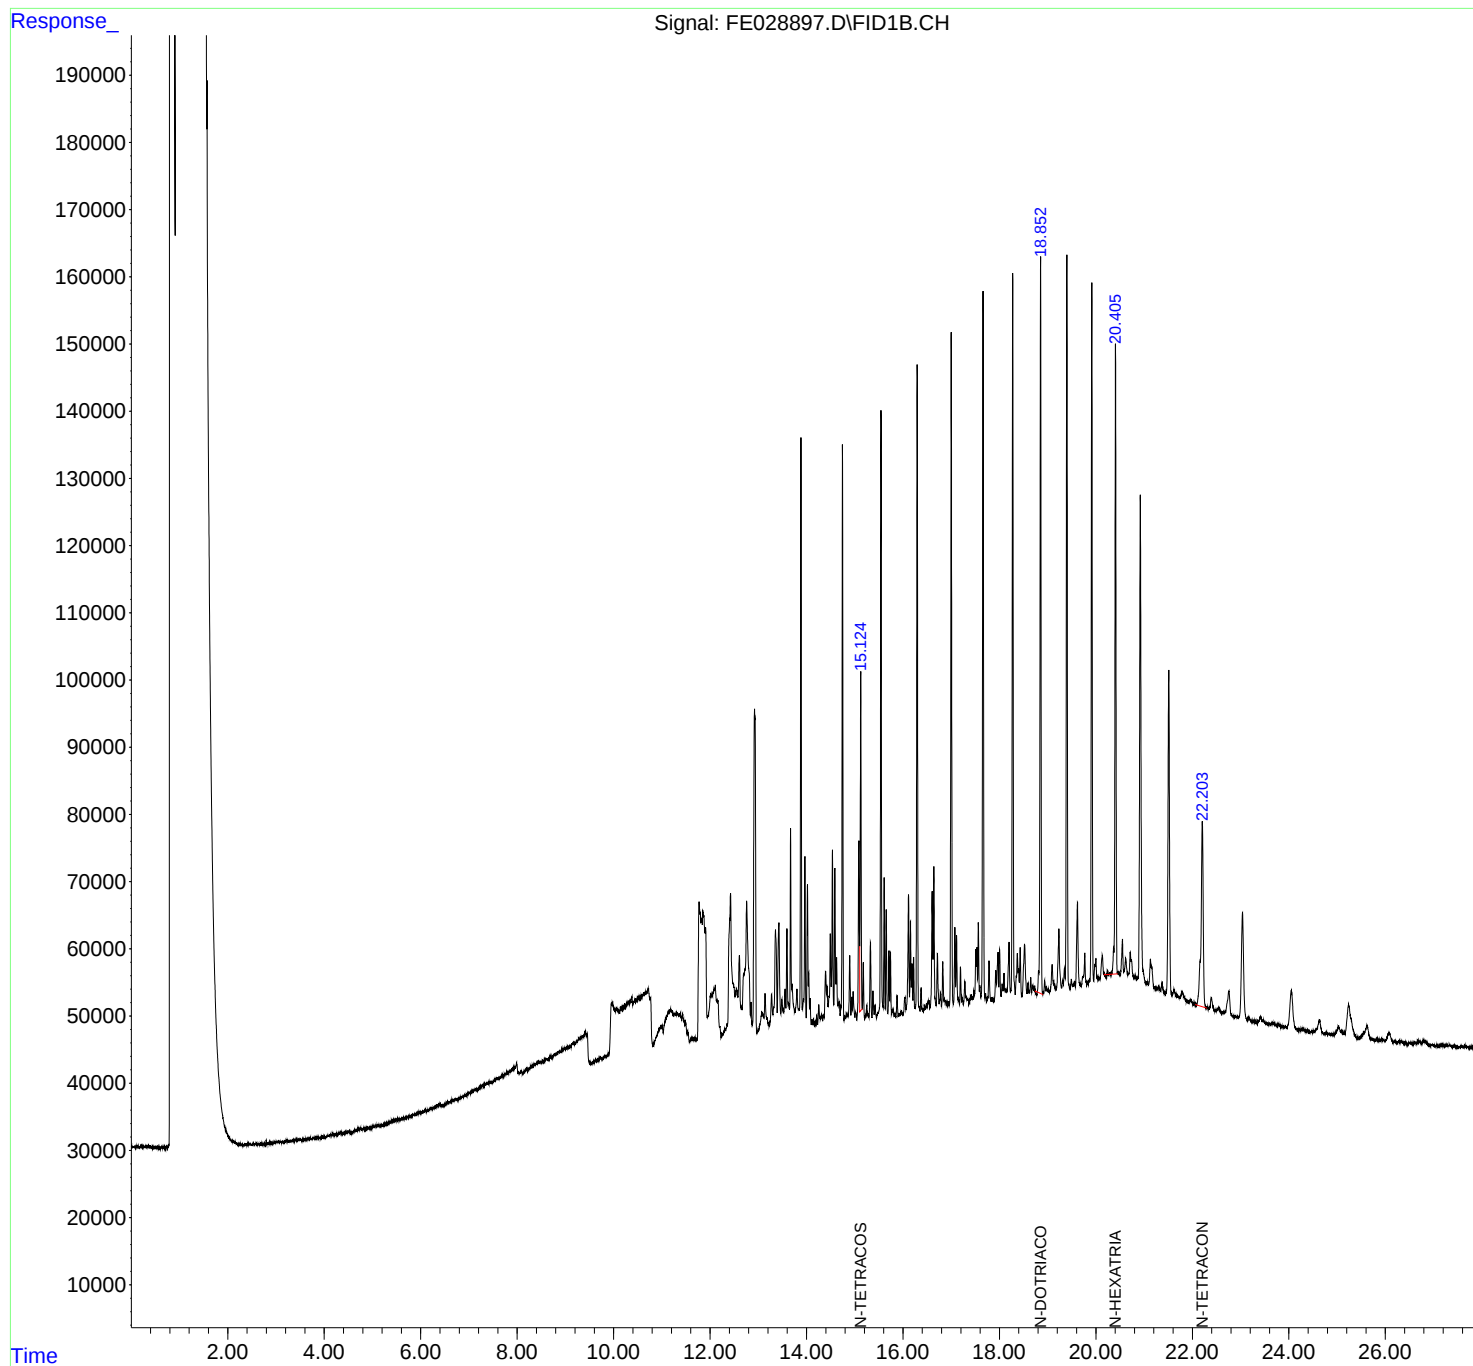

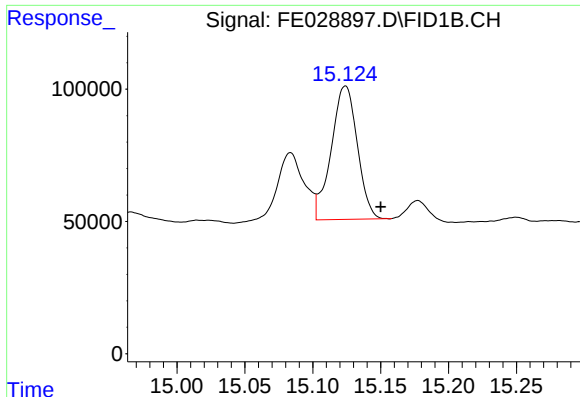


#10 N-TETRACOSANE

R.T.: 15.124 min
Delta R.T.: -0.026 min
Response: 675434
Conc: 3.87 ug/ml

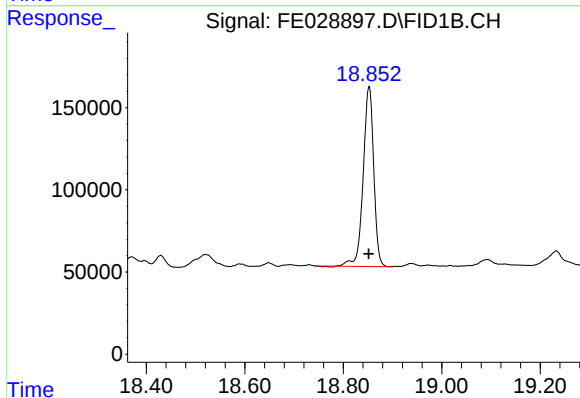


#12 N-DOTRIACONTANE

R.T.: 18.852 min
Delta R.T.: 0.000 min
Response: 1626766
Conc: 12.52 ug/ml

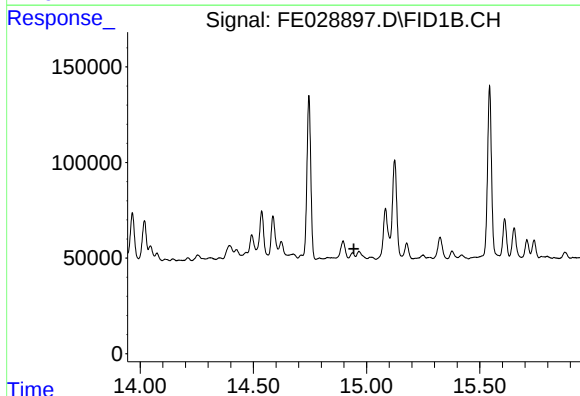


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.944 min
Response: 0
Conc: N.D.

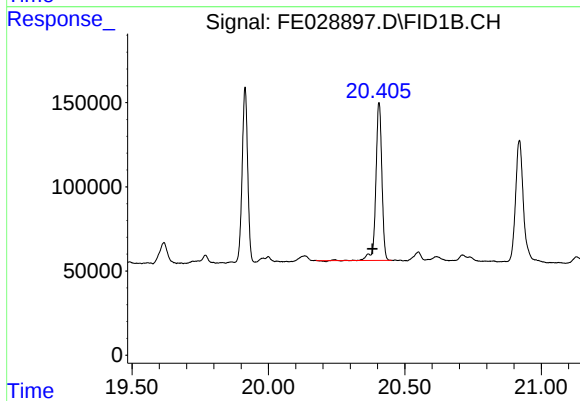

#14 N-HEXATRIACONTANE

R.T.: 20.405 min
Delta R.T.: 0.025 min
Response: 1442495
Conc: 14.28 ug/ml

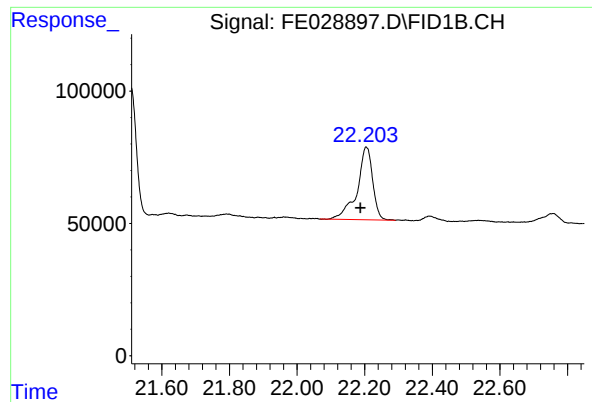

#15 N-TETRACONTANE

R.T.: 22.205 min
Delta R.T.: 0.018 min
Response: 876381
Conc: 12.12 ug/ml