

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101121\
 Data File : FE034423.D
 Signal(s) : FID1B.CH
 Acq On : 11 Oct 2021 10:30
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Oct 11 14:54:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
 Quant Title :
 QLast Update : Fri Oct 08 16:08:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.631	17014271	49.896 ug/ml
Target Compounds			
2) N-DECANE	4.399	19897919	51.795 ug/ml
3) N-DODECANE	6.404	19968067	52.301 ug/ml
4) N-TETRADECANE	8.196	20190238	51.315 ug/ml
5) N-HEXADECANE	9.793	19961401	50.540 ug/ml
6) N-OCTADECANE	11.233	20090601	50.057 ug/ml
7) N-EICOSANE	12.540	19992995	49.692 ug/ml
8) N-DOCOSANE	13.736	19621087	49.926 ug/ml
10) N-TETRACOSANE	14.837	19453406	49.957 ug/ml
11) N-HEXACOSANE	15.855	19031425	49.887 ug/ml
12) N-OCTACOSANE	16.801	18606130	49.289 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101121\
Data File : FE034423.D
Signal(s) : FID1B.CH
Acq On : 11 Oct 2021 10:30
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Oct 11 14:54:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100821.M
Quant Title :
QLast Update : Fri Oct 08 16:08:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

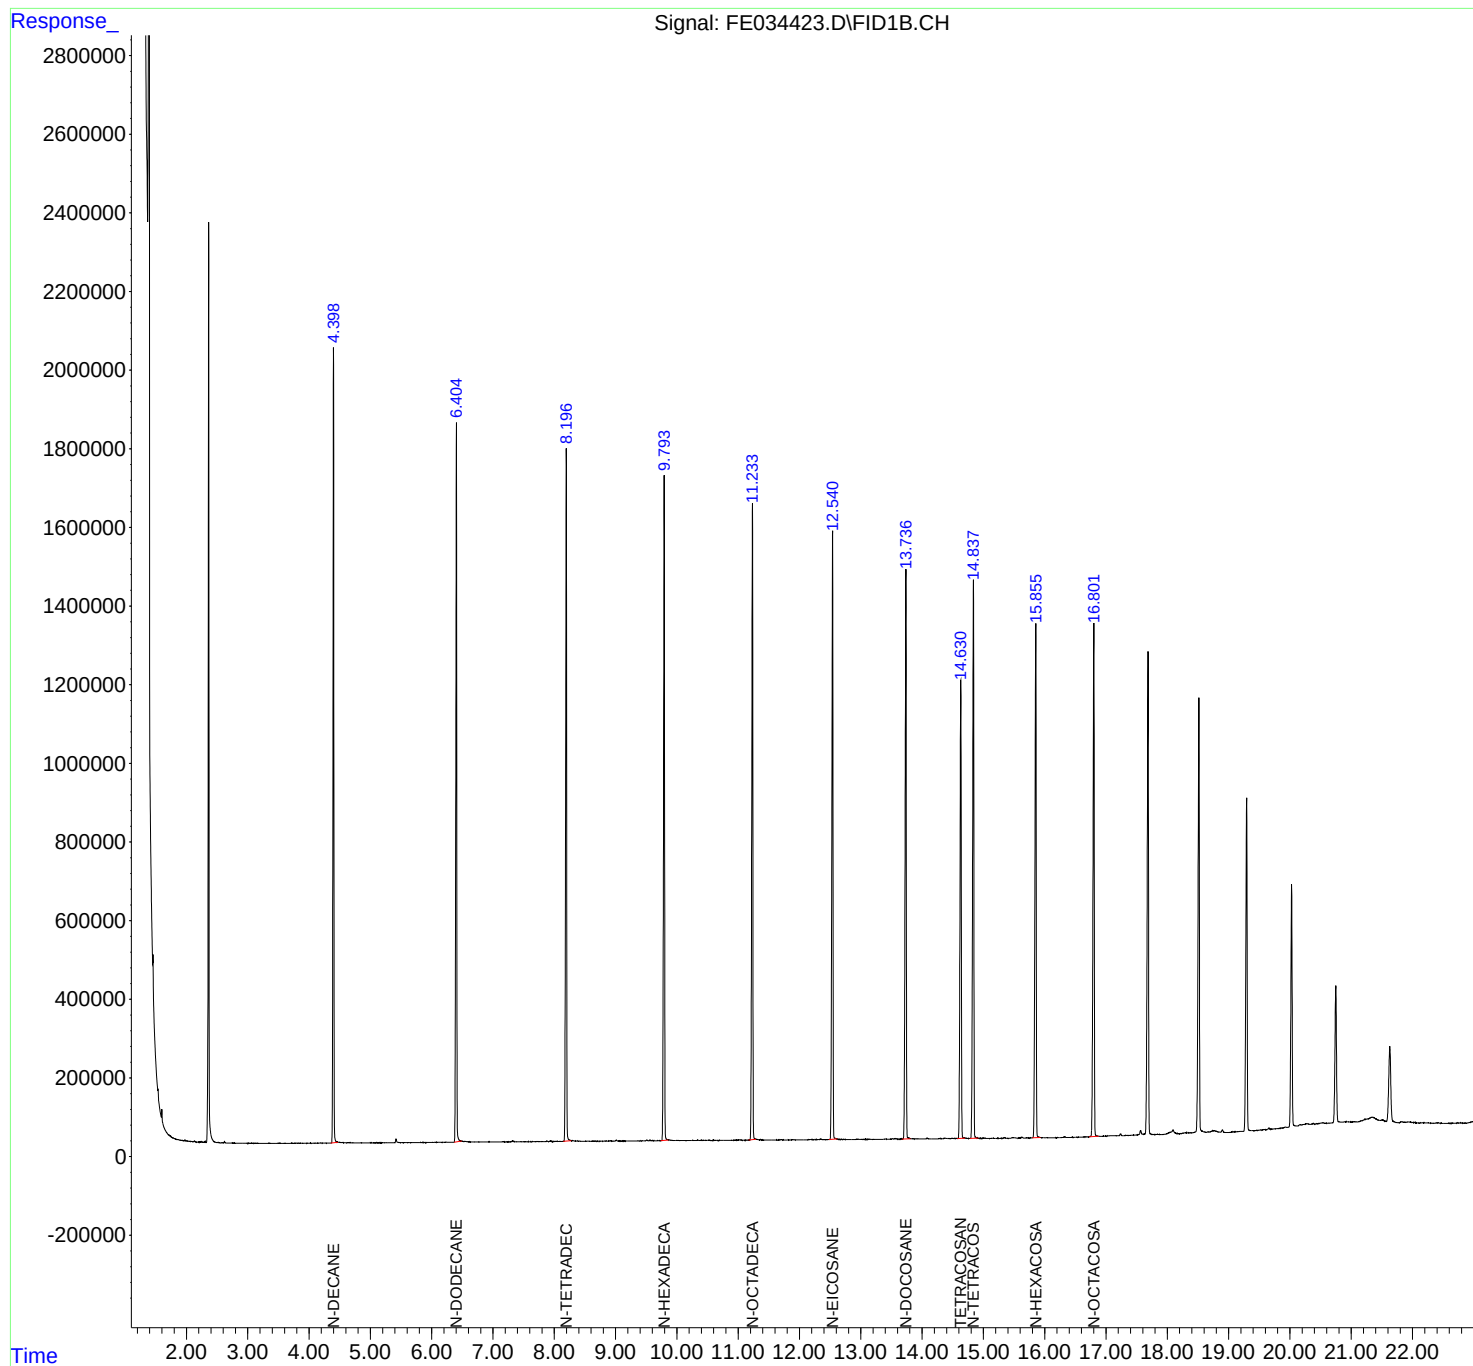


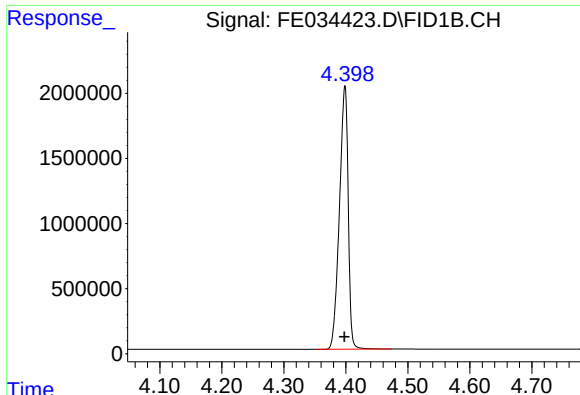

#2 N-DECANE


R.T.: 4.399 min
Delta R.T.: 0.000 min
Response: 19897919
Conc: 51.79 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

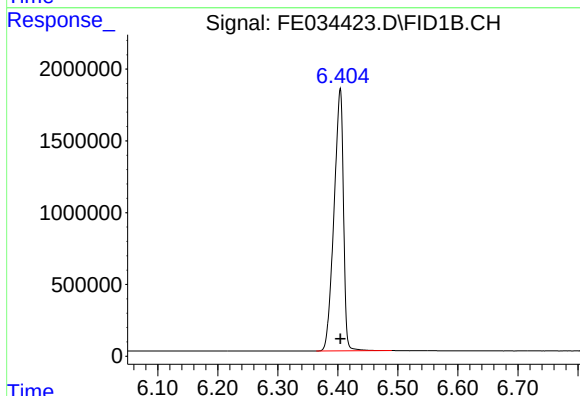


#3 N-DODECANE

R.T.: 6.404 min
Delta R.T.: 0.000 min
Response: 19968067
Conc: 52.30 ug/ml

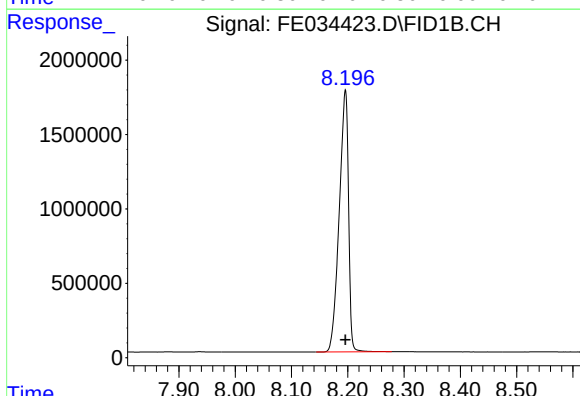


#4 N-TETRADECANE

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 20190238
Conc: 51.32 ug/ml

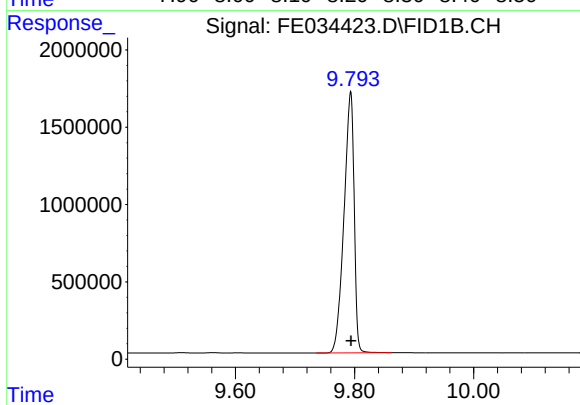

#5 N-HEXADECANE


R.T.: 9.793 min
Delta R.T.: 0.000 min
Response: 19961401
Conc: 50.54 ug/ml

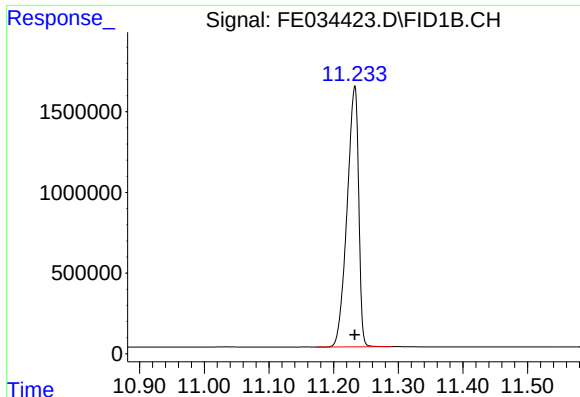

#6 N-OCTADECANE


R.T.: 11.233 min
Delta R.T.: 0.000 min
Response: 20090601
Conc: 50.06 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

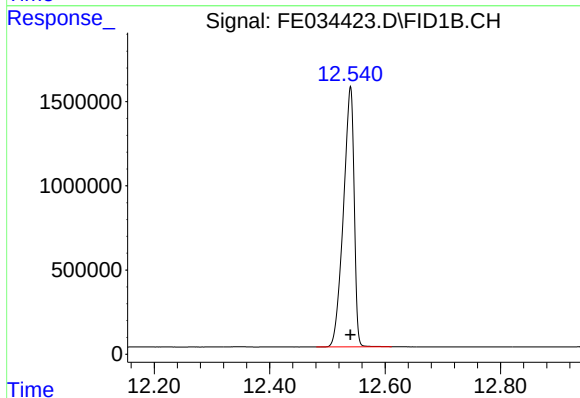


#7 N-EICOSANE

R.T.: 12.540 min
Delta R.T.: 0.000 min
Response: 19992995
Conc: 49.69 ug/ml

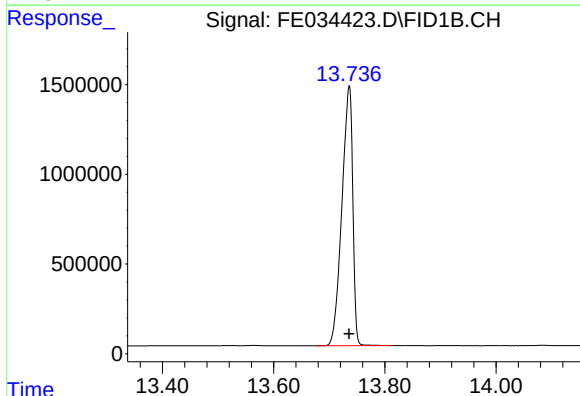


#8 N-DOCOSANE

R.T.: 13.736 min
Delta R.T.: 0.000 min
Response: 19621087
Conc: 49.93 ug/ml

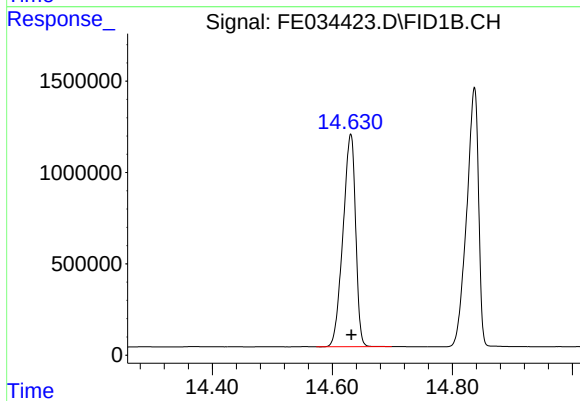

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.631 min
Delta R.T.: -0.001 min
Response: 17014271
Conc: 49.90 ug/ml

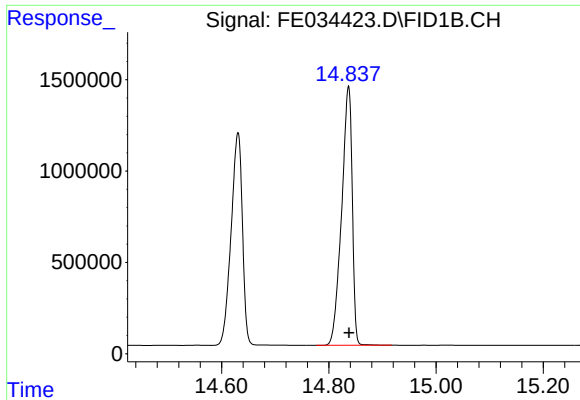

#10 N-TETRACOSANE


R.T.: 14.837 min
Delta R.T.: 0.000 min
Response: 19453406
Conc: 49.96 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

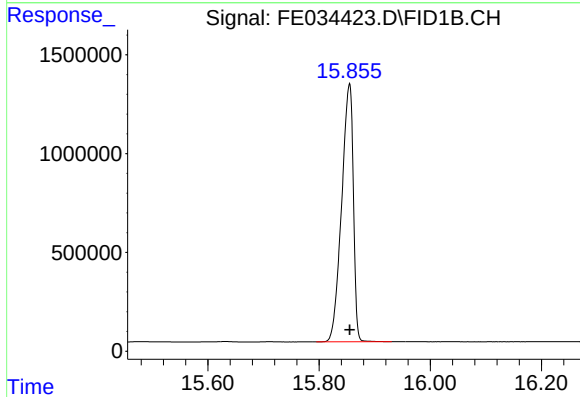

#11 N-HEXACOSANE

R.T.: 15.855 min
Delta R.T.: 0.000 min
Response: 19031425
Conc: 49.89 ug/ml

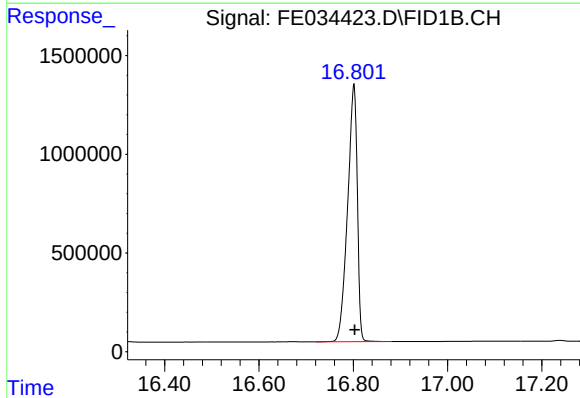

#12 N-OCTACOSANE

R.T.: 16.801 min
Delta R.T.: -0.002 min
Response: 18606130
Conc: 49.29 ug/ml