

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101123AL\
Data File : FE044797.D
Signal(s) : FID1B.ch
Acq On : 12 Oct 2023 00:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 12 01:16:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.910	74167	0.501 ug/ml
20) T	n-Hexatriacontane (C36)	20.434	71458	0.493 ug/ml
22) T	n-Tetracontane (C40)	22.104	231734	1.468 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101123AL\
Data File : FE044797.D
Signal(s) : FID1B.ch
Acq On : 12 Oct 2023 00:15
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 12 01:16:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 11:06:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

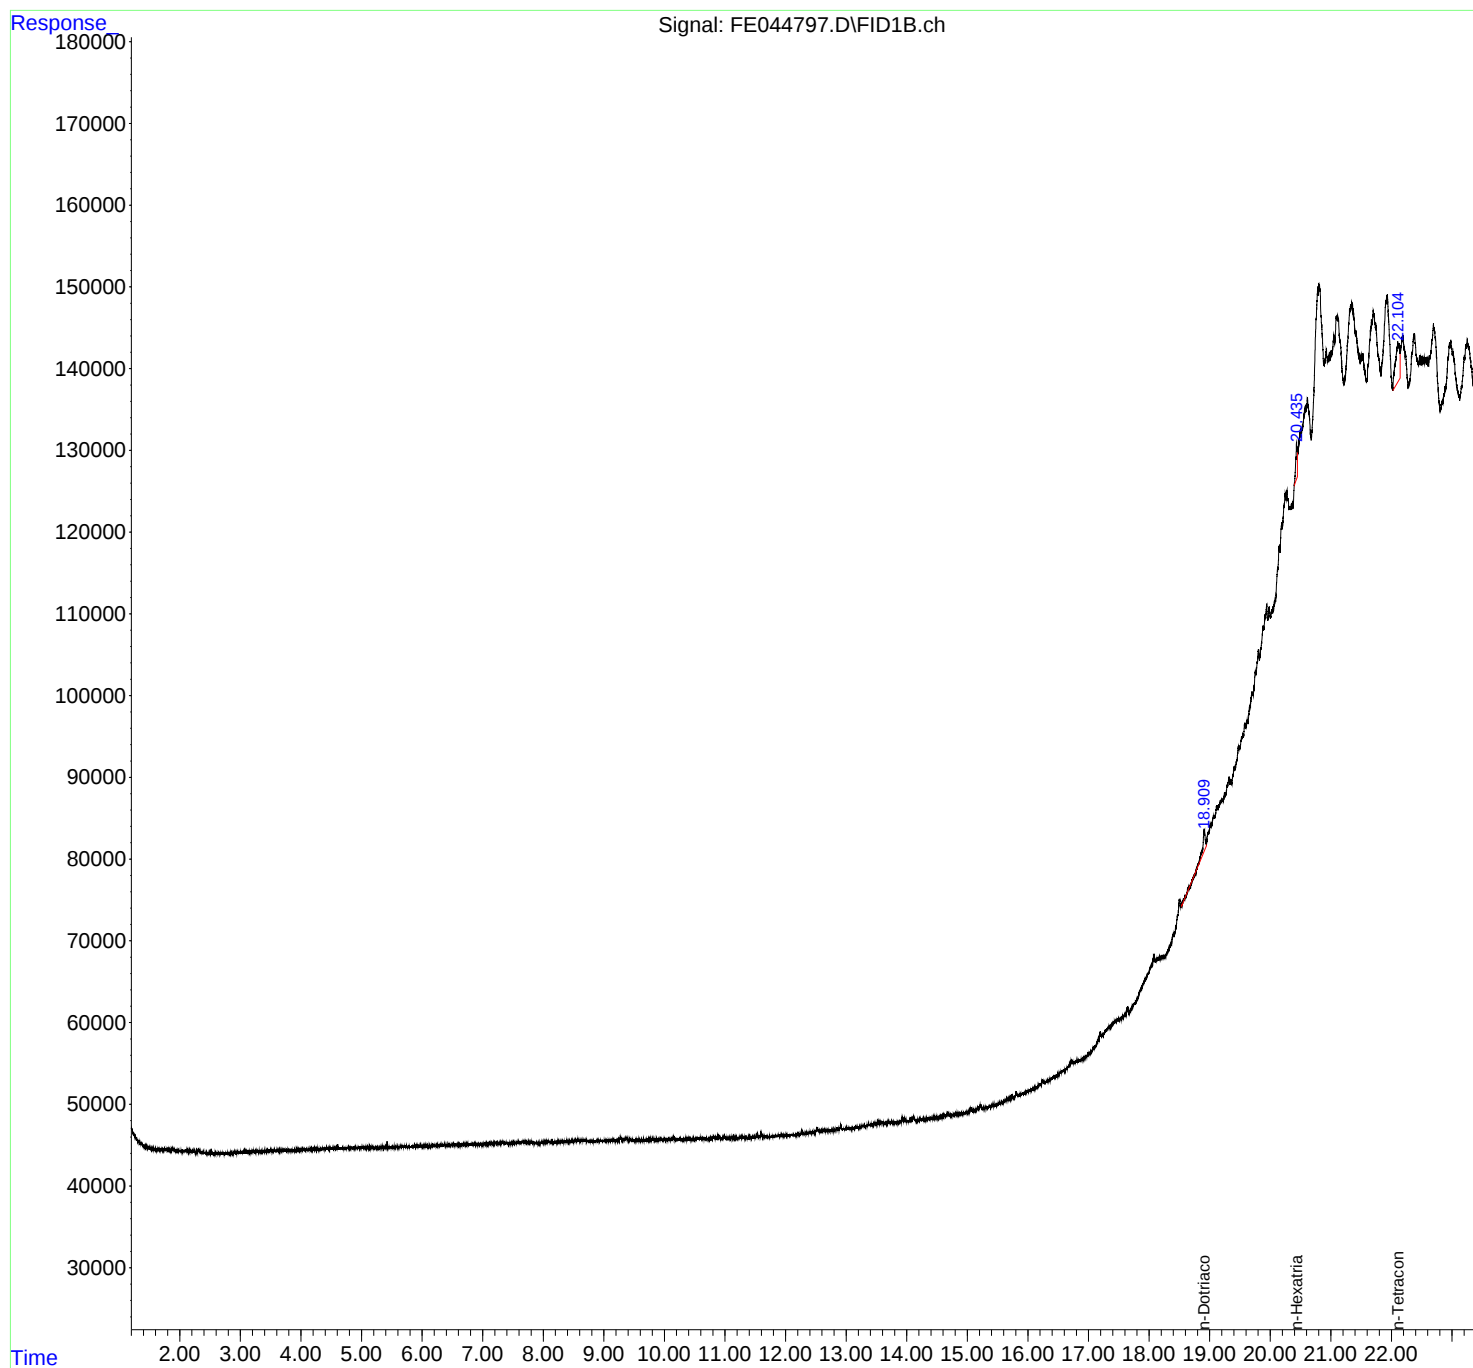


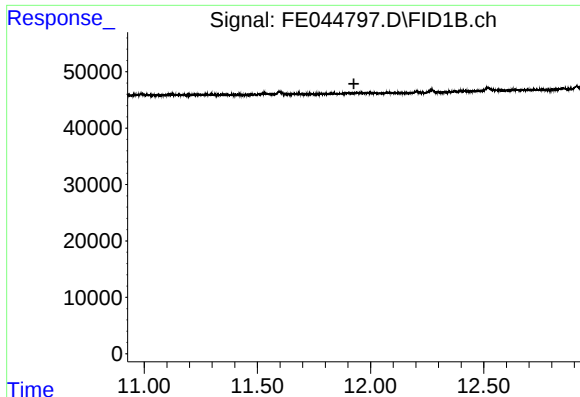

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.926 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

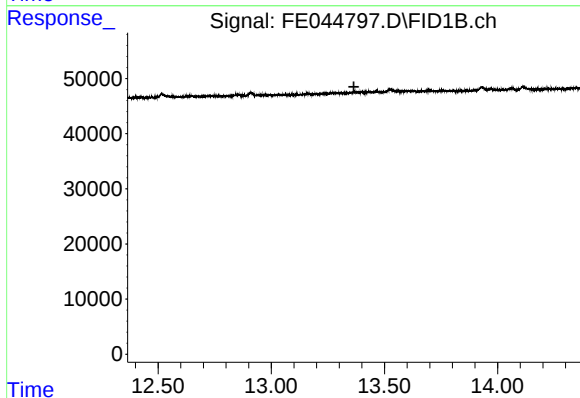


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.365 min
Response: 0
Conc: N.D.

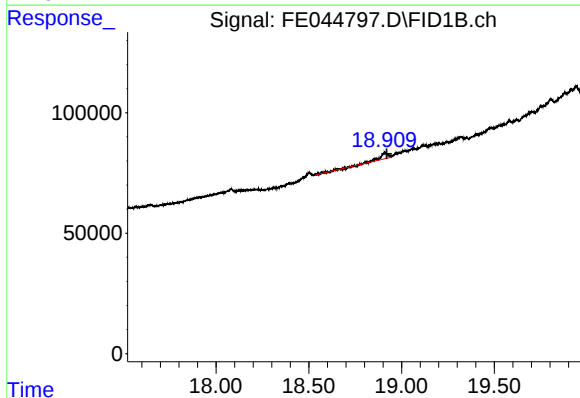


#18 n-Dotriacontane (C32)

R.T.: 18.910 min
Delta R.T.: -0.010 min
Response: 74167
Conc: 0.50 ug/ml

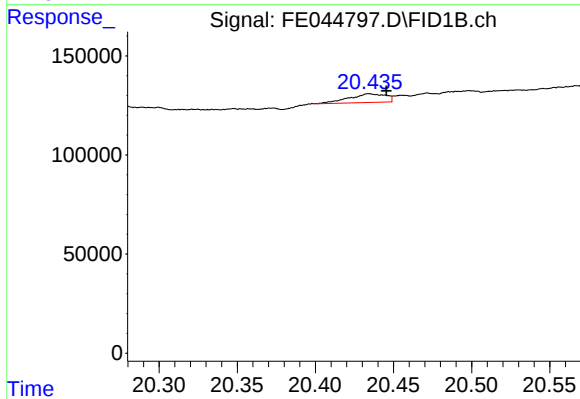

#20 n-Hexatriacontane (C36)

R.T.: 20.434 min
Delta R.T.: -0.011 min
Response: 71458
Conc: 0.49 ug/ml

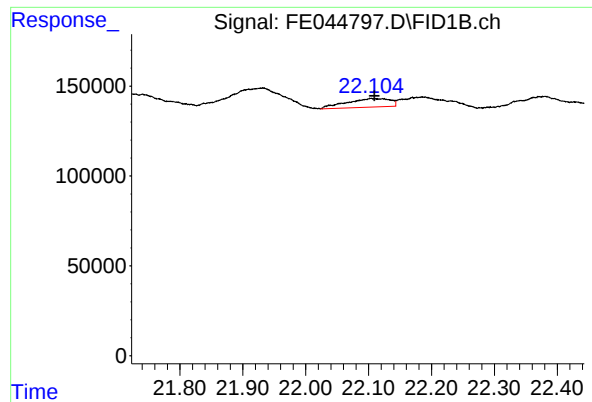

#22 n-Tetracontane (C40)

R.T.: 22.104 min
Delta R.T.: -0.005 min
Response: 231734
Conc: 1.47 ug/ml

Instrument :

FID_E

ClientSampleId :