

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101124\
 Data File : FE050605.D
 Signal(s) : FID1B.ch
 Acq On : 10 Oct 2024 23:30
 Operator : YP\AJ
 Sample : PB164026BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_E
ClientSampleId :
 PB164026BL

Integration File: autoint1.e
 Quant Time: Oct 11 03:56:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101124.M
 Quant Title :
 QLast Update : Thu Oct 10 13:46:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.941	2399803	17.221 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101124\
Data File : FE050605.D
Signal(s) : FID1B.ch
Acq On : 10 Oct 2024 23:30
Operator : YP\AJ
Sample : PB164026BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB164026BL

Integration File: autoint1.e
Quant Time: Oct 11 03:56:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101124.M
Quant Title :
QLast Update : Thu Oct 10 13:46:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

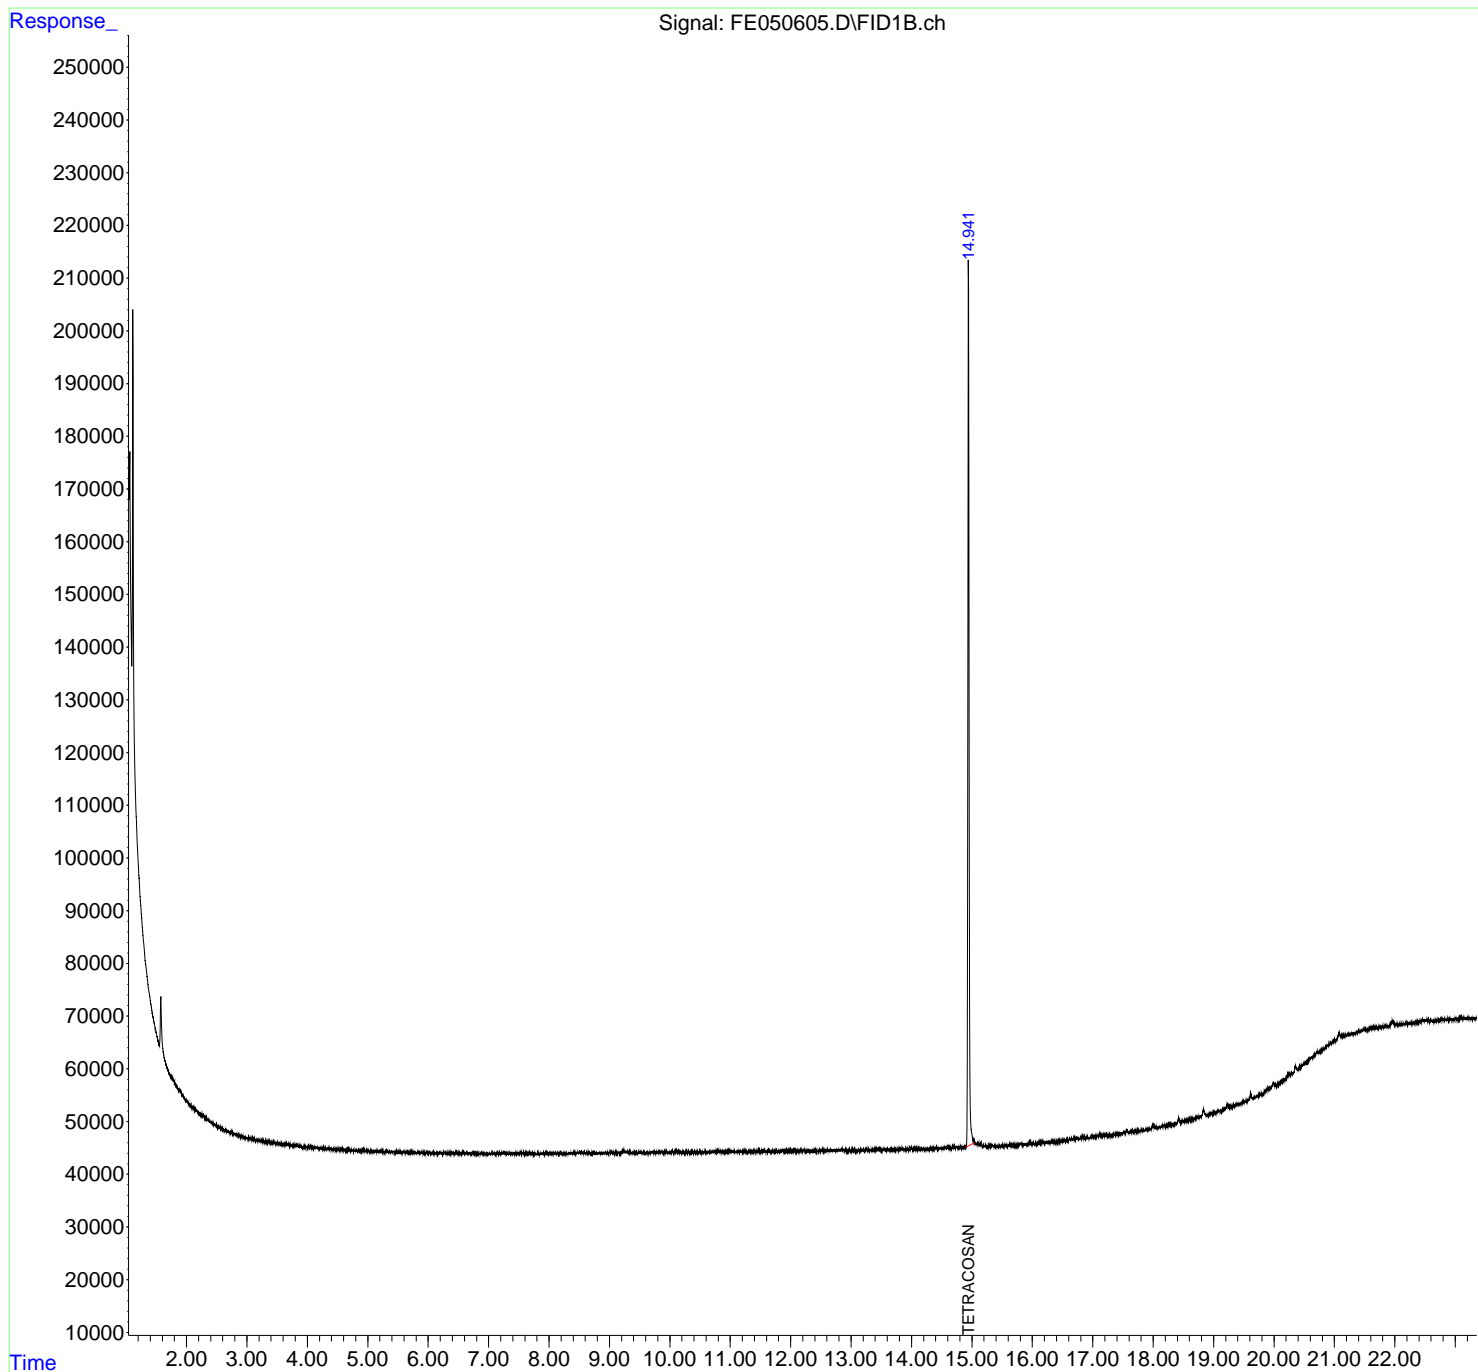

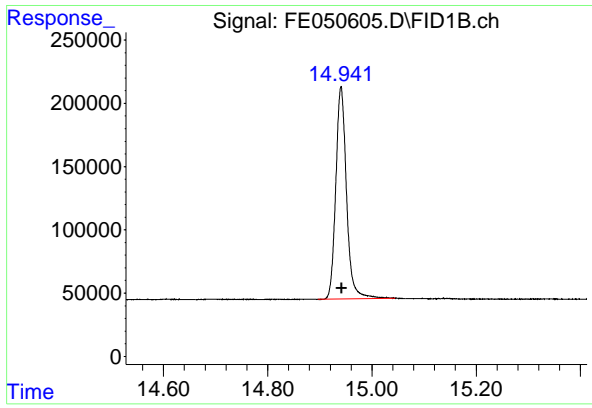

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.941 min
Delta R.T.: -0.001 min
Response: 2399803
Conc: 17.22 ug/ml

Instrument :
FID_E
ClientSampleId :
PB164026BL