

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101222\
Data File : FE038089.D
Signal(s) : FID1B.ch
Acq On : 12 Oct 2022 13:45
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 13 05:13:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.425	2756493	19.717 ug/ml
12) N-OCTACOSANE	16.822	2763641	19.641 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101222\
Data File : FE038089.D
Signal(s) : FID1B.ch
Acq On : 12 Oct 2022 13:45
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 13 05:13:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

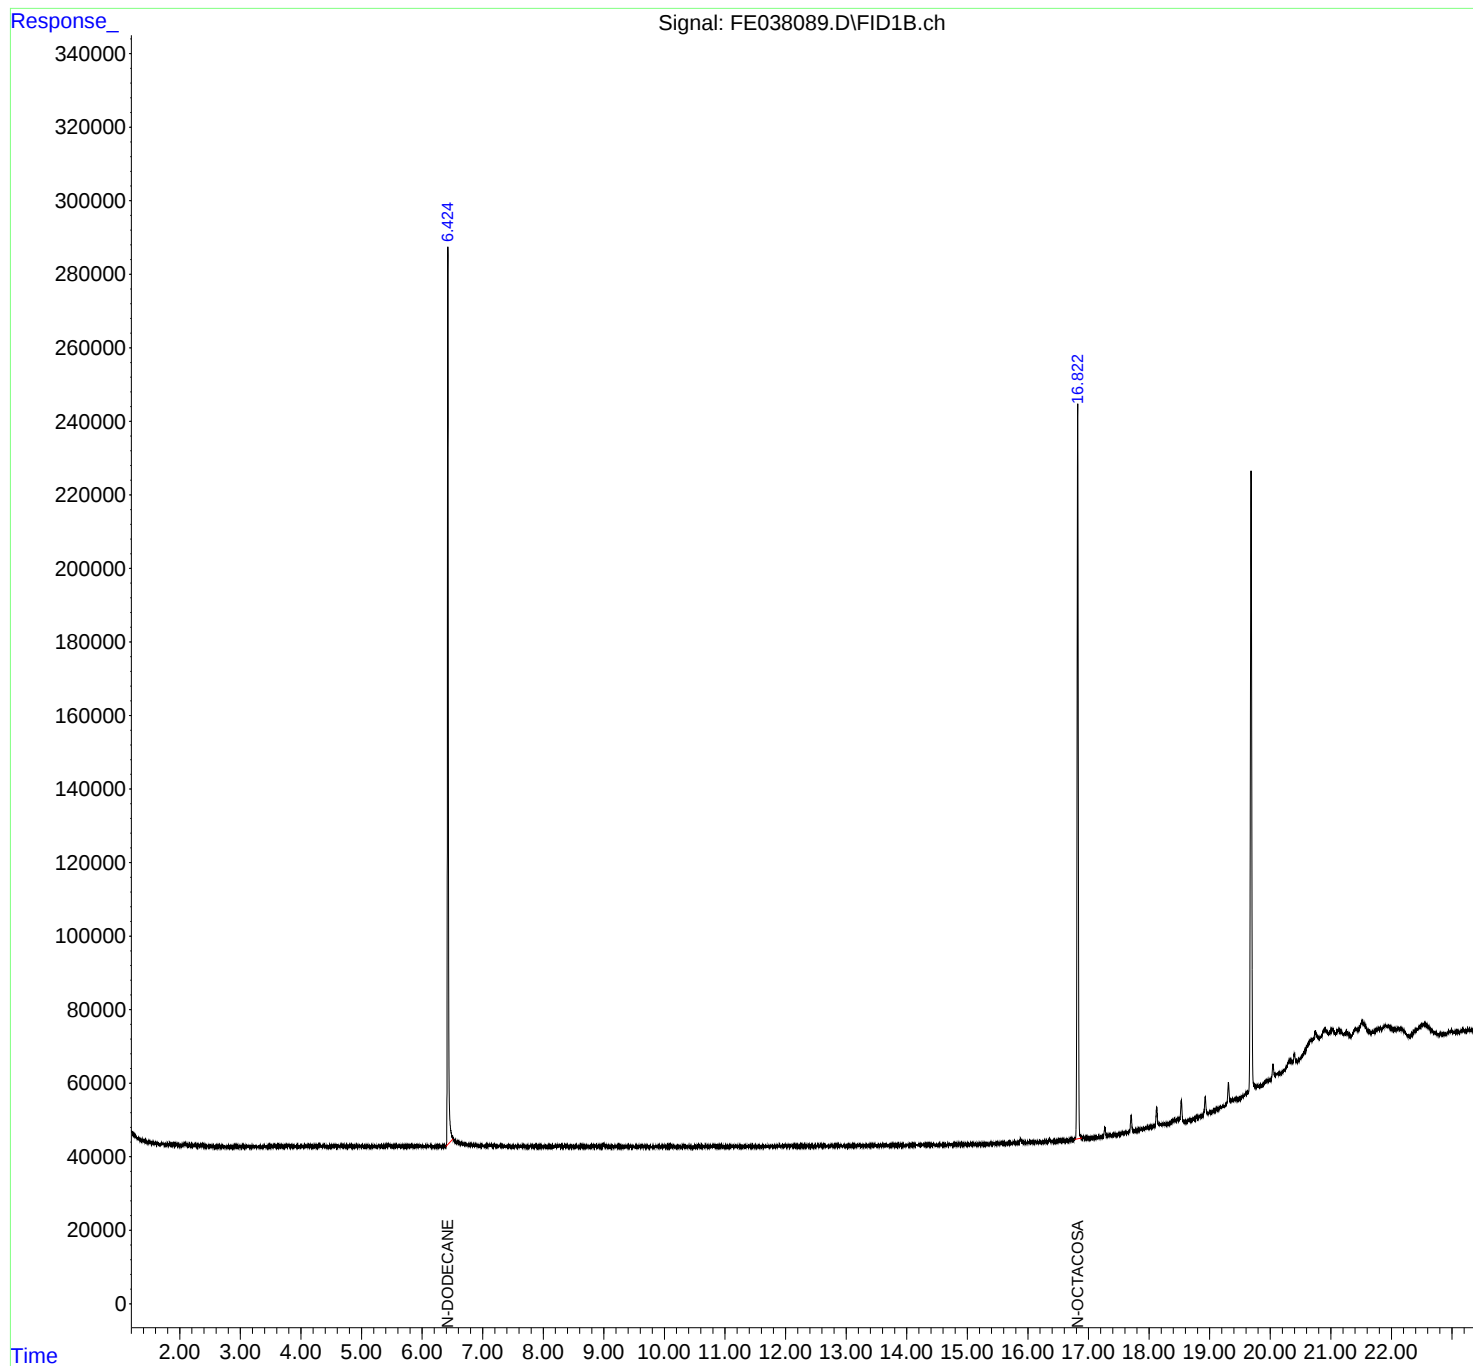


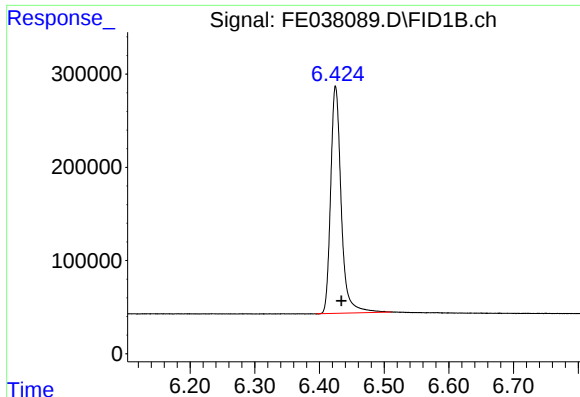

#3 N-DODECANE


R.T.: 6.425 min
Delta R.T.: -0.009 min
Response: 2756493
Conc: 19.72 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

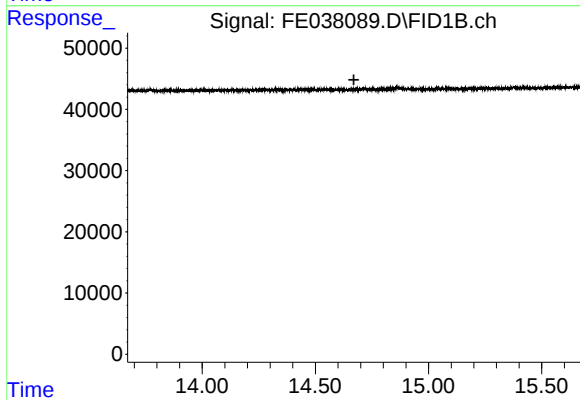

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.670 min
Response: 0
Conc: N.D.

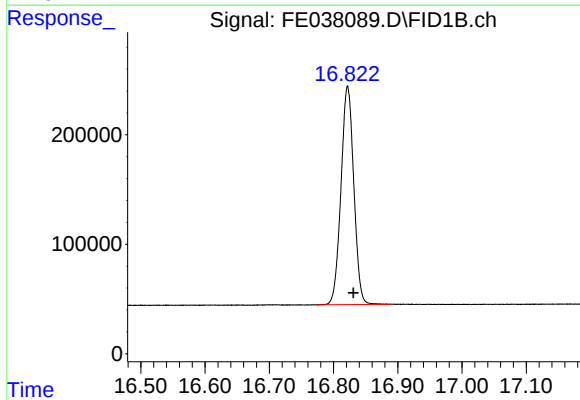

#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.009 min
Response: 2763641
Conc: 19.64 ug/ml