

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101222\
Data File : FE038090.D
Signal(s) : FID1B.ch
Acq On : 12 Oct 2022 16:33
Operator : YP\AJ
Sample : N5068-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B5(15-16)

Integration File: autoint1.e
Quant Time: Oct 13 05:13:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	4975030	38.302 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101222\
Data File : FE038090.D
Signal(s) : FID1B.ch
Acq On : 12 Oct 2022 16:33
Operator : YP\AJ
Sample : N5068-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B5(15-16)

Integration File: autoint1.e
Quant Time: Oct 13 05:13:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

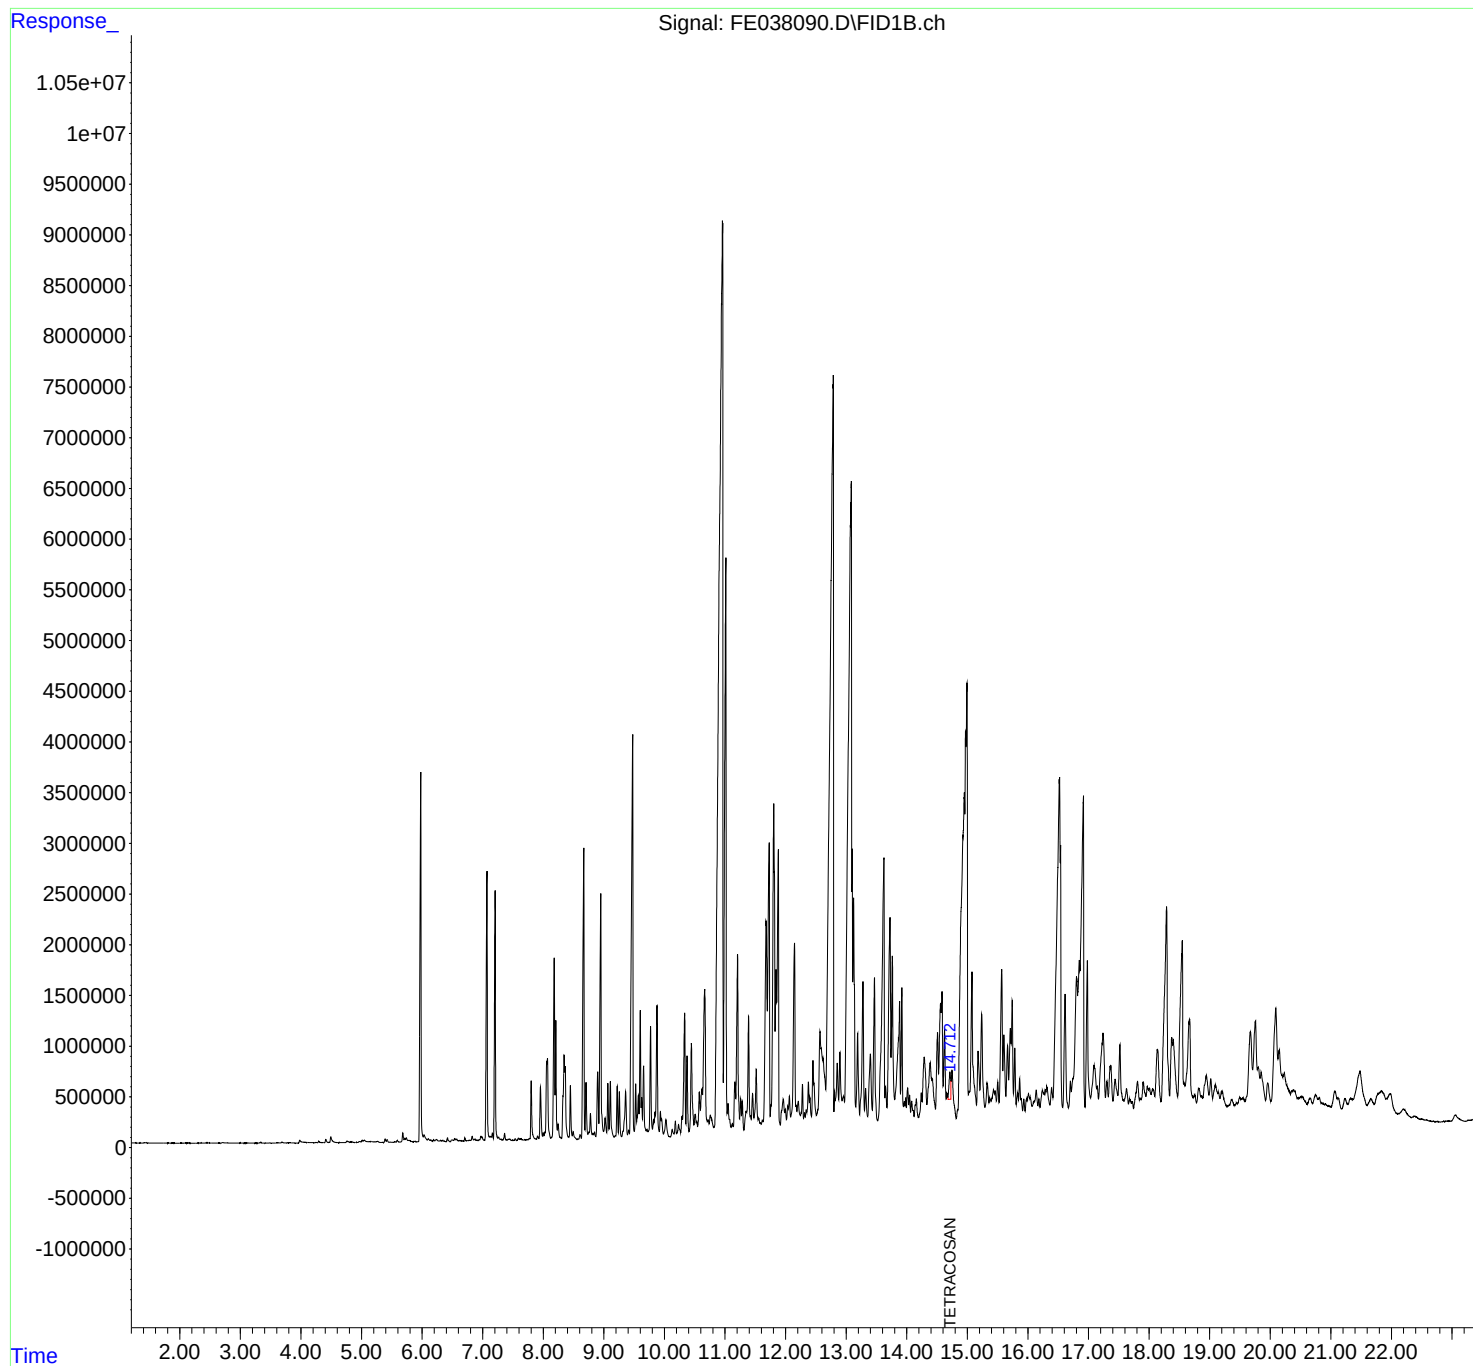

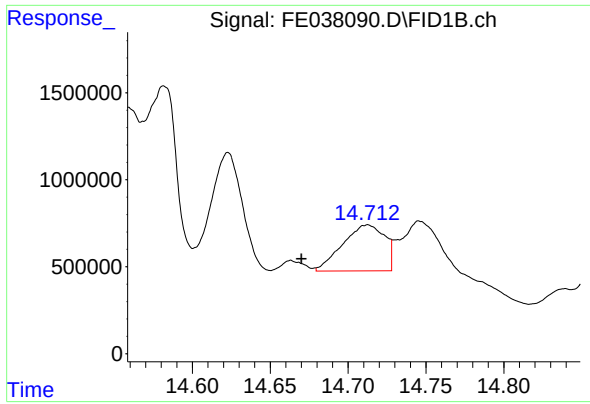

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: 0.042 min
Response: 4975030
Conc: 38.30 ug/ml

Instrument :
FID_E
ClientSampleId :
B5(15-16)