

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE101222\  
Data File : FE038100.D  
Signal(s) : FID1B.ch  
Acq On : 12 Oct 2022 21:47  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Oct 13 05:14:46 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE100522.M  
Quant Title :  
QLast Update : Wed Oct 05 16:55:43 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.665 | 2431082  | 18.716 ug/ml |

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE101222\  
Data File : FE038100.D  
Signal(s) : FID1B.ch  
Acq On : 12 Oct 2022 21:47  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Oct 13 05:14:46 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE100522.M  
Quant Title :  
QLast Update : Wed Oct 05 16:55:43 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

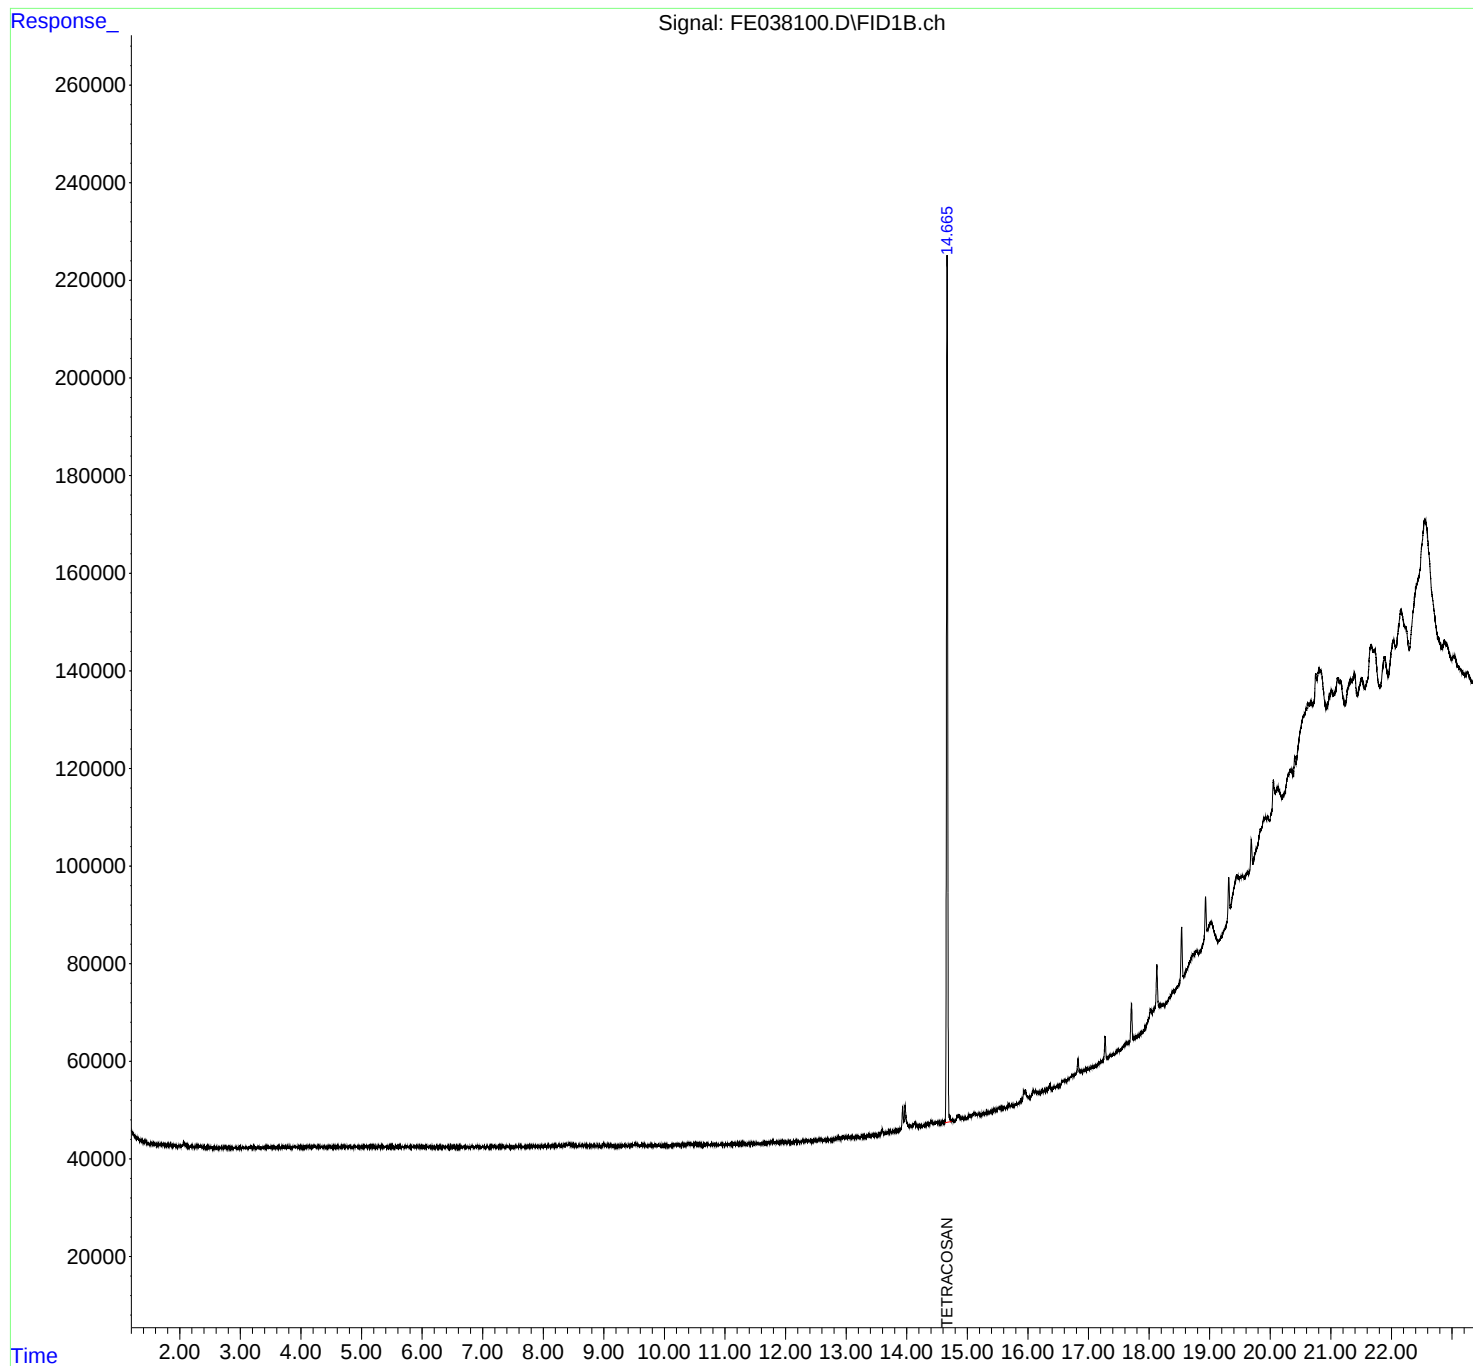

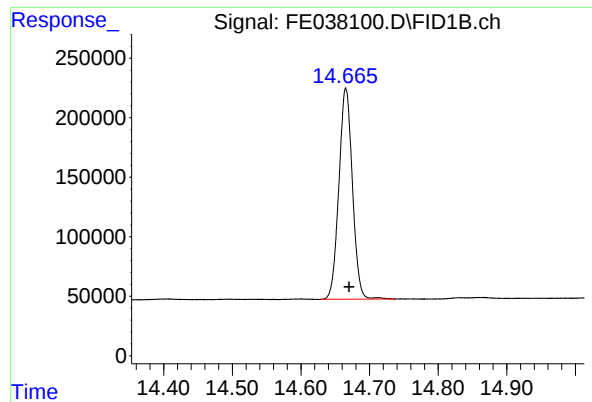

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.665 min  
Delta R.T.: -0.005 min  
Response: 2431082  
Conc: 18.72 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK