

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101322\
Data File : FE038106.D
Signal(s) : FID1B.ch
Acq On : 13 Oct 2022 10:29
Operator : YP\AJ
Sample : N5068-09 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B6(20-21)

Integration File: autoint1.e
Quant Time: Oct 13 12:50:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.659	297939	2.294 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101322\
Data File : FE038106.D
Signal(s) : FID1B.ch
Acq On : 13 Oct 2022 10:29
Operator : YP\AJ
Sample : N5068-09 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
B6(20-21)

Integration File: autoint1.e
Quant Time: Oct 13 12:50:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE100522.M
Quant Title :
QLast Update : Wed Oct 05 16:55:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

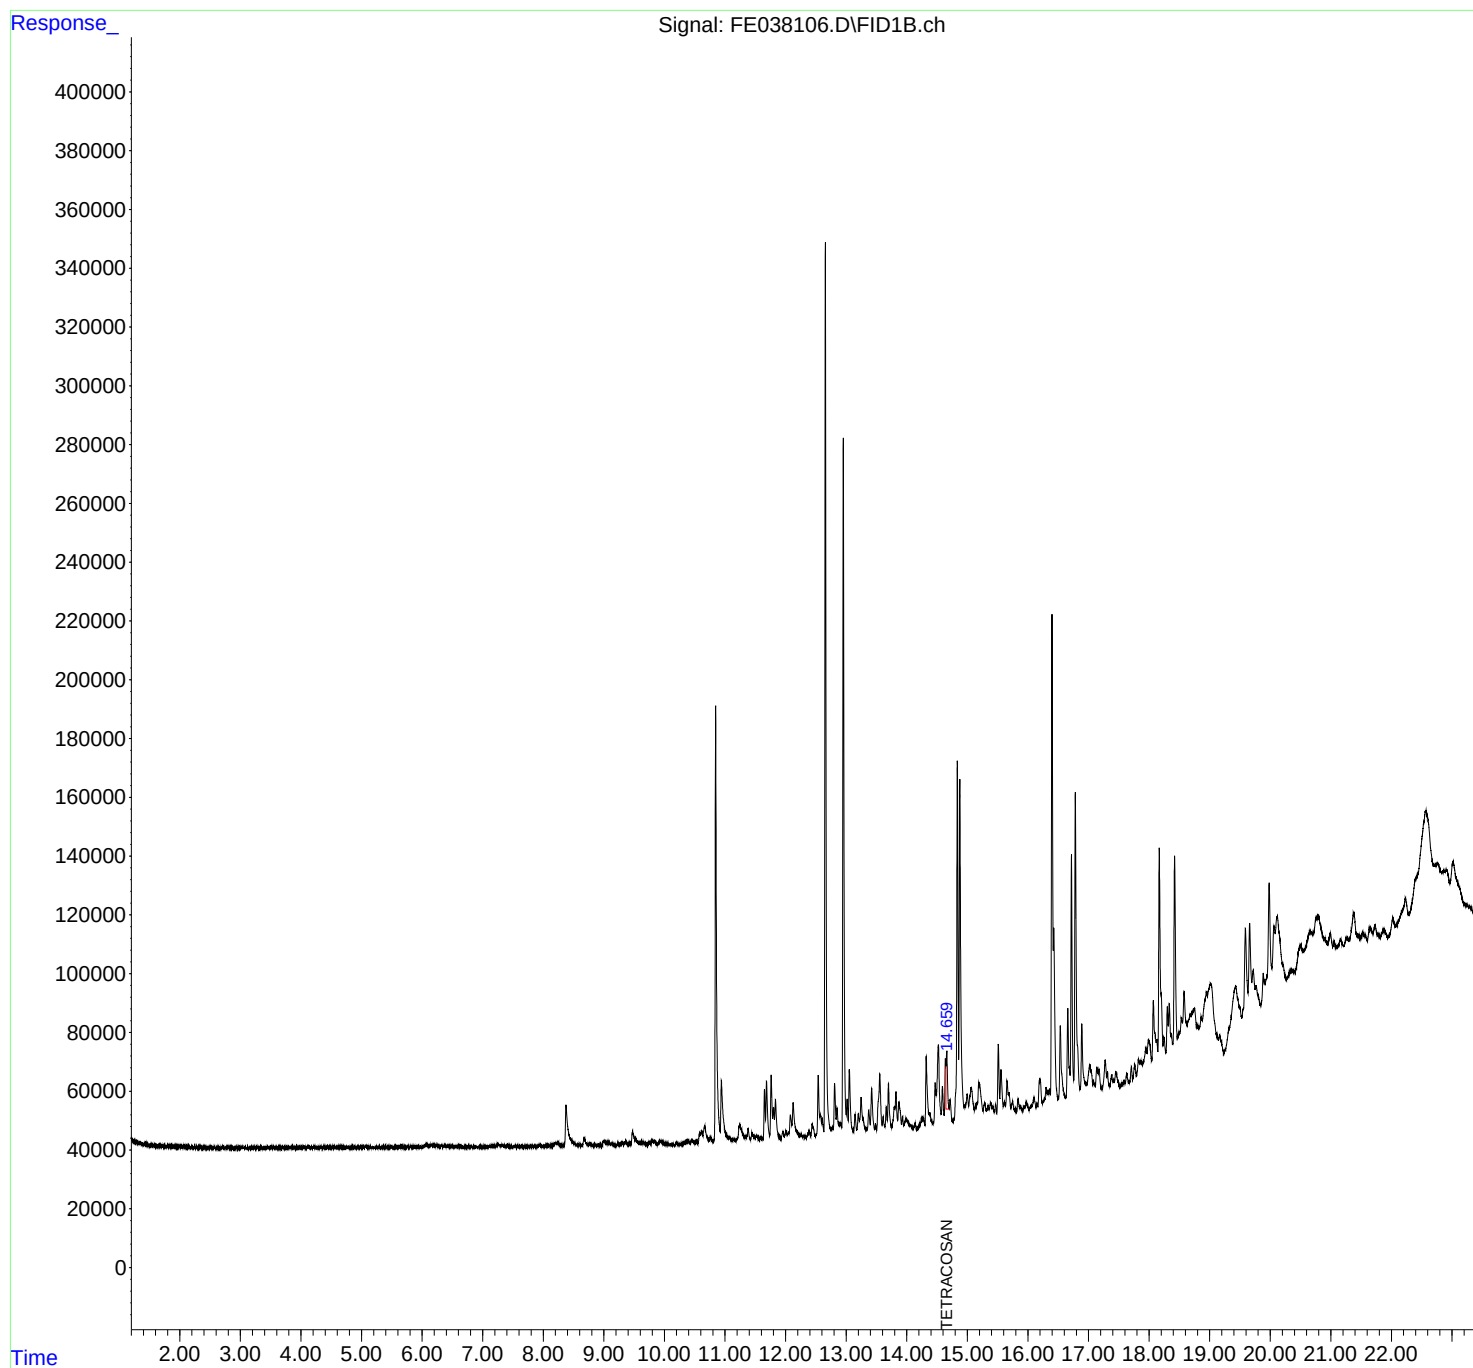

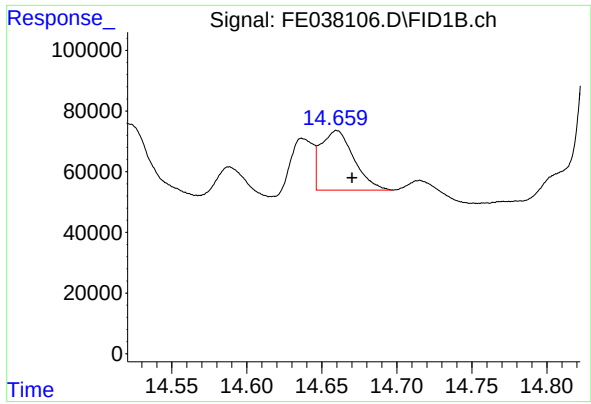

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.659 min
Delta R.T.: -0.011 min
Response: 297939
Conc: 2.29 ug/ml

Instrument :
FID_E
ClientSampleId :
B6(20-21)