

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101424\
Data File : FE050636.D
Signal(s) : FID1B.ch
Acq On : 14 Oct 2024 13:19
Operator : YP\AJ
Sample : PB164063BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB164063BL

Integration File: autoint1.e
Quant Time: Oct 15 03:04:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101124.M
Quant Title :
QLast Update : Thu Oct 10 13:46:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.945	2440437	17.513 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101424\
Data File : FE050636.D
Signal(s) : FID1B.ch
Acq On : 14 Oct 2024 13:19
Operator : YP\AJ
Sample : PB164063BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB164063BL

Integration File: autoint1.e
Quant Time: Oct 15 03:04:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101124.M
Quant Title :
QLast Update : Thu Oct 10 13:46:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

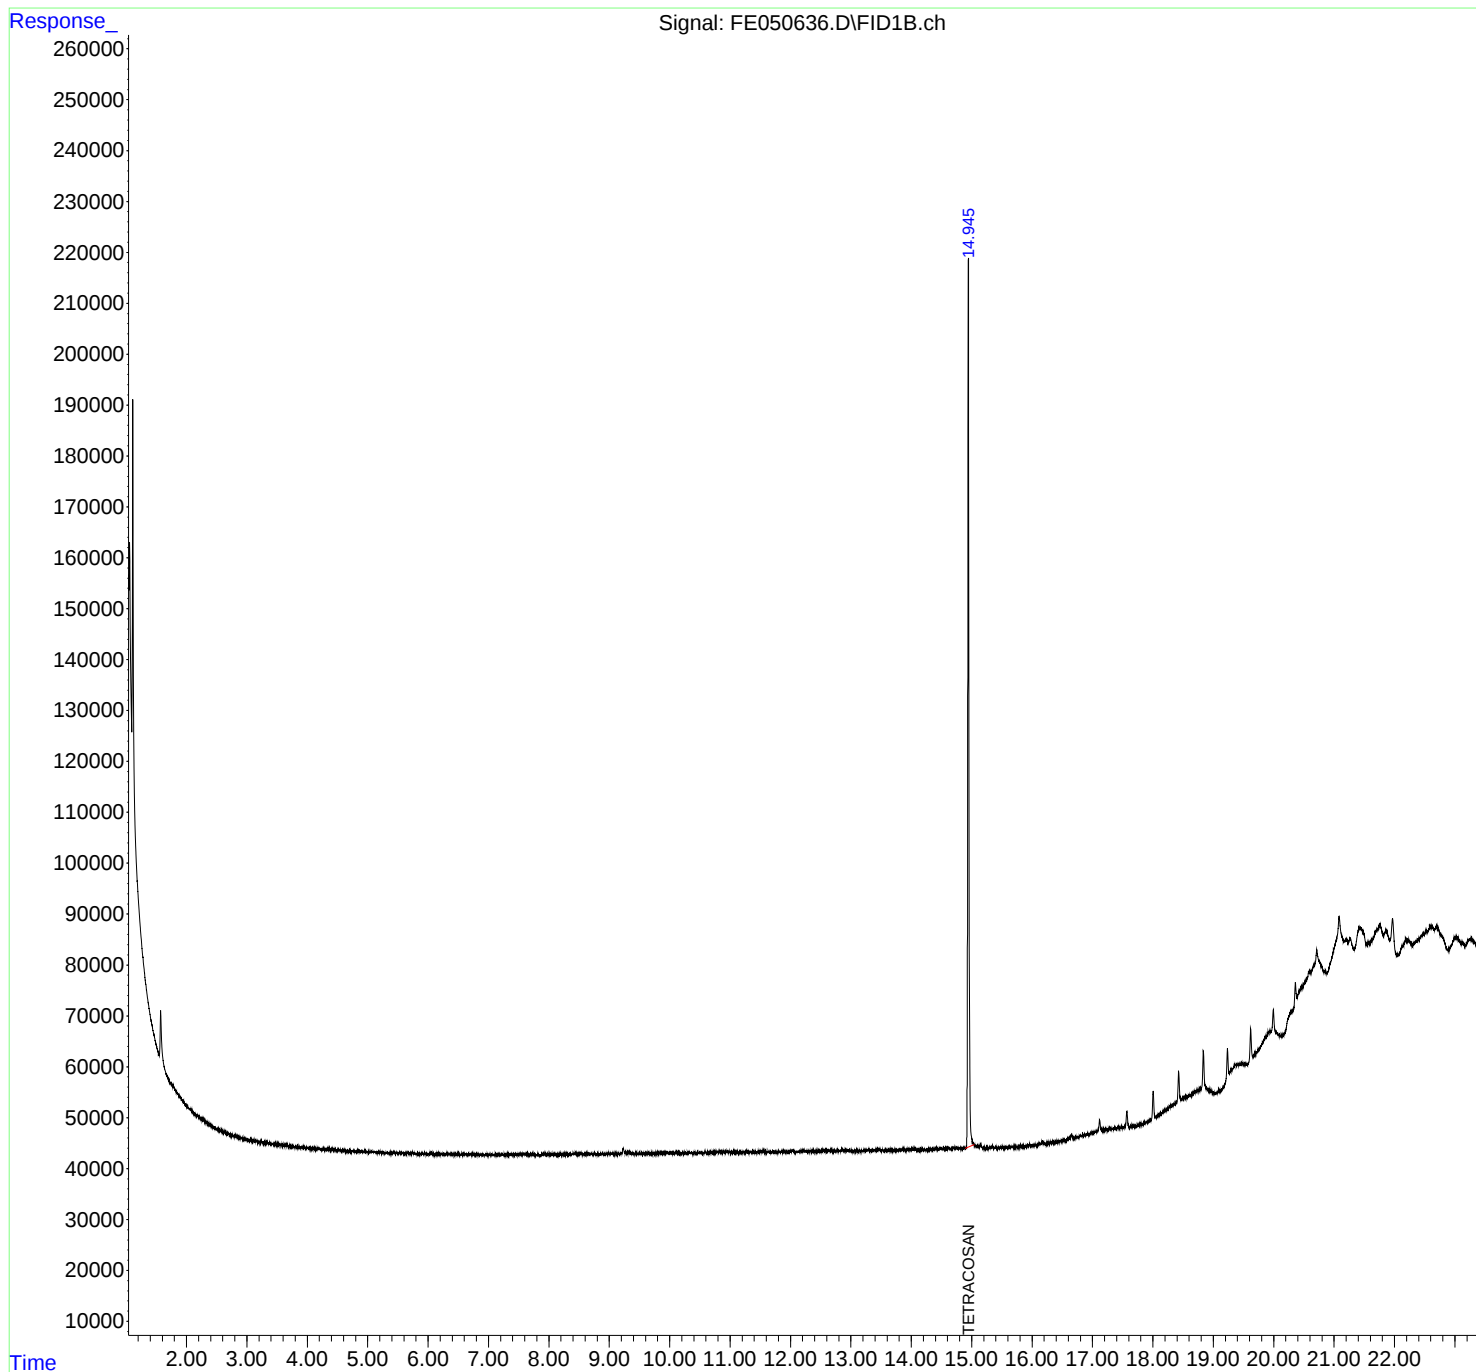

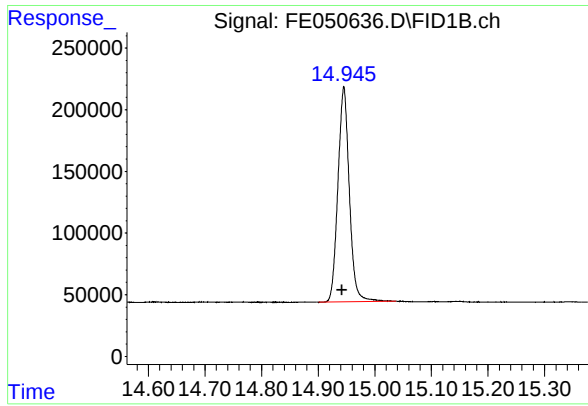

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.945 min
Delta R.T.: 0.003 min
Response: 2440437
Conc: 17.51 ug/ml

Instrument :
FID_E
ClientSampleId :
PB164063BL