

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101520\
 Data File : FE032983.D
 Signal(s) : FID1B.CH
 Acq On : 15 Oct 2020 9:05
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 16 01:27:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101420.M
 Quant Title :
 QLast Update : Wed Oct 14 02:47:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.657	17040679	55.024 ug/ml
Target Compounds				
2)	N-DECANE	4.409	19424136	56.339 ug/ml
3)	N-DODECANE	6.419	19667269	57.055 ug/ml
4)	N-TETRADECANE	8.211	19623668	56.789 ug/ml
5)	N-HEXADECANE	9.812	19997387	56.372 ug/ml
6)	N-OCTADECANE	11.254	20060728	55.632 ug/ml
7)	N-EICOSANE	12.562	19827017	55.261 ug/ml
8)	N-DOCOSANE	13.761	19517313	54.869 ug/ml
10)	N-TETRACOSANE	14.864	19506449	54.738 ug/ml
11)	N-HEXACOSANE	15.883	19121190	54.576 ug/ml
12)	N-OCTACOSANE	16.834	18823268	54.314 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101520\
Data File : FE032983.D
Signal(s) : FID1B.CH
Acq On : 15 Oct 2020 9:05
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 16 01:27:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101420.M
Quant Title :
QLast Update : Wed Oct 14 02:47:05 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

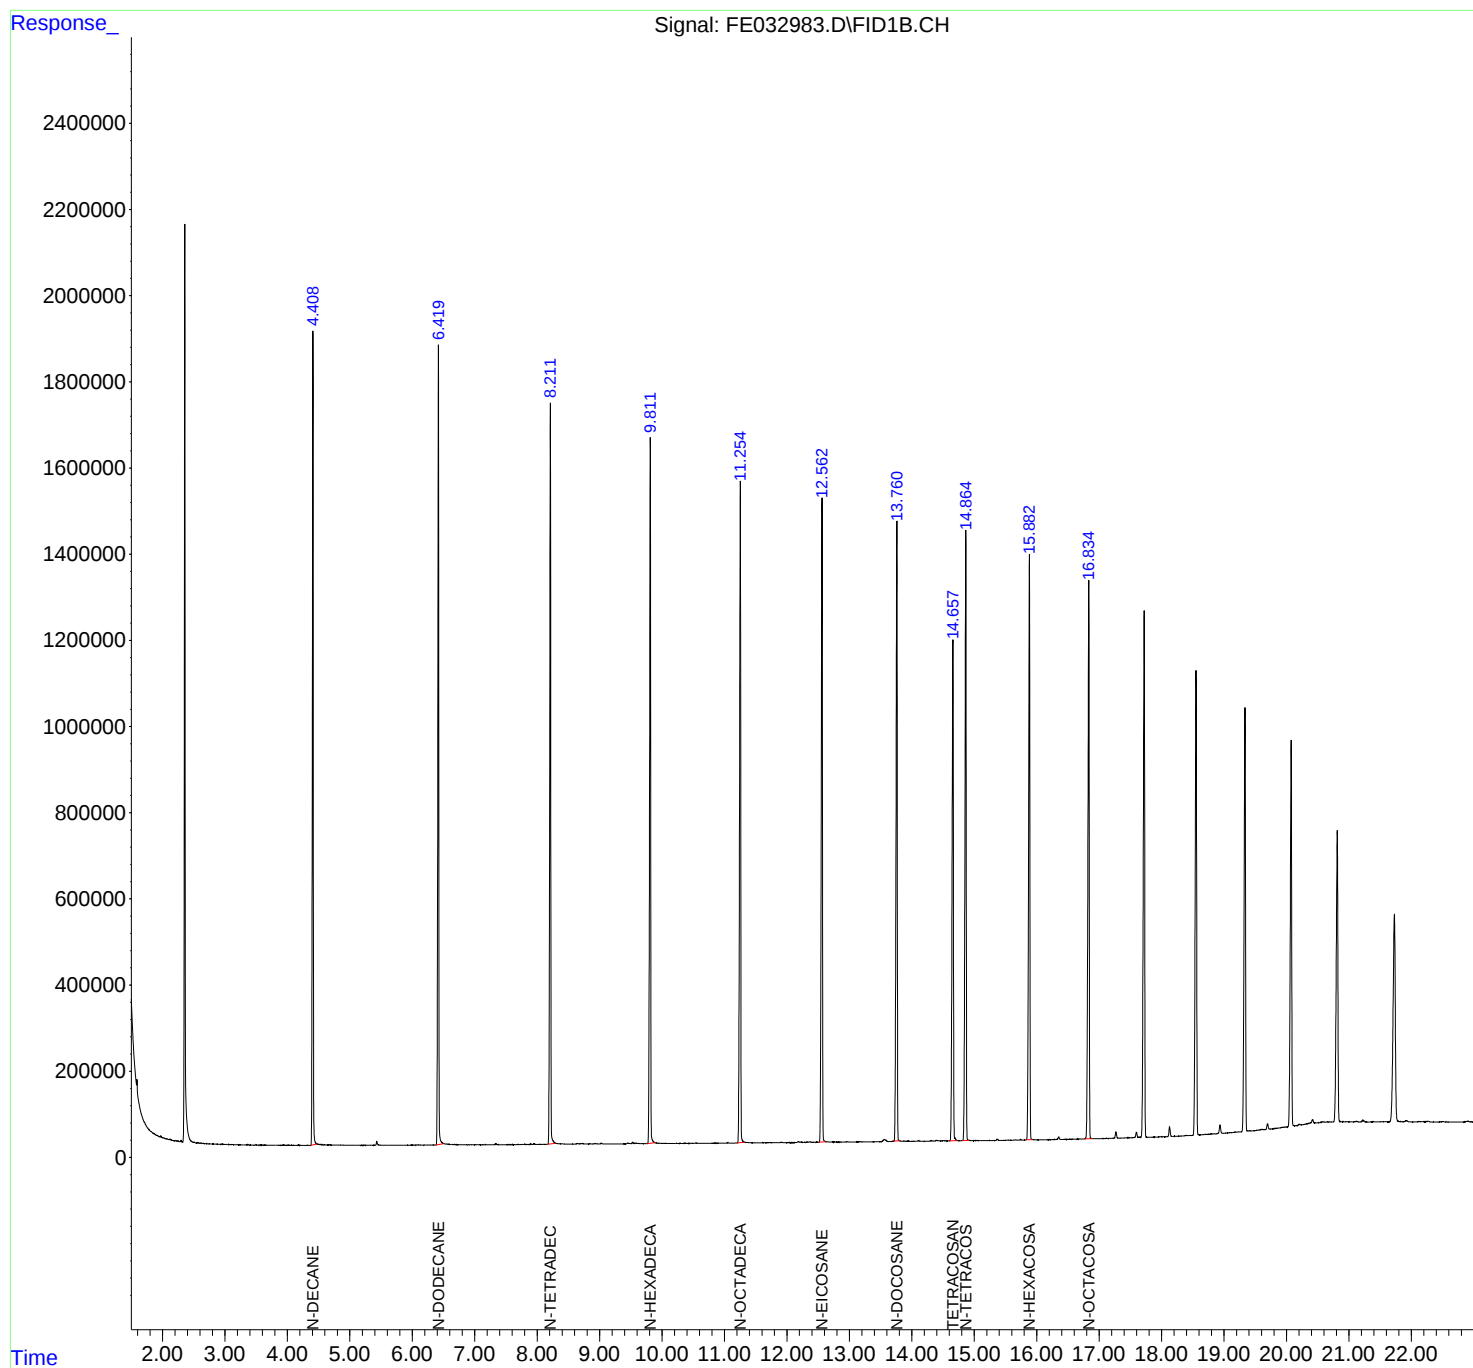

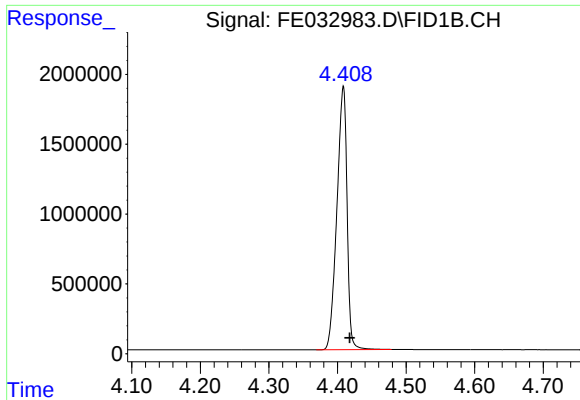


#2 N-DECANE

R.T.: 4.409 min
Delta R.T.: -0.009 min
Response: 19424136
Conc: 56.34 ug/ml

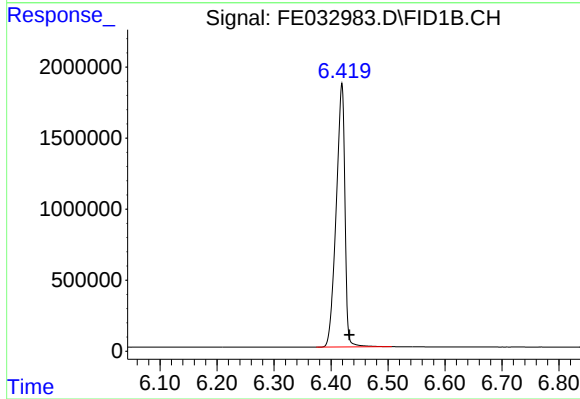


#3 N-DODECANE

R.T.: 6.419 min
Delta R.T.: -0.013 min
Response: 19667269
Conc: 57.06 ug/ml

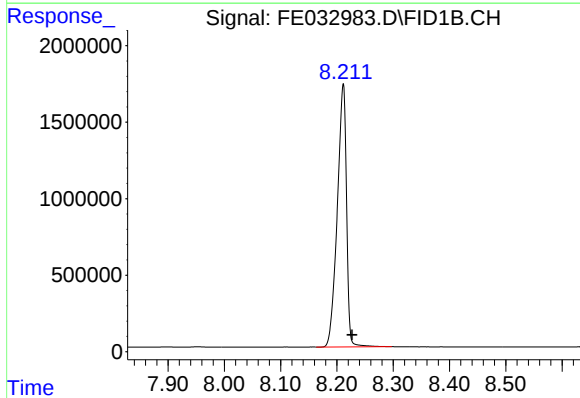


#4 N-TETRADECANE

R.T.: 8.211 min
Delta R.T.: -0.016 min
Response: 19623668
Conc: 56.79 ug/ml

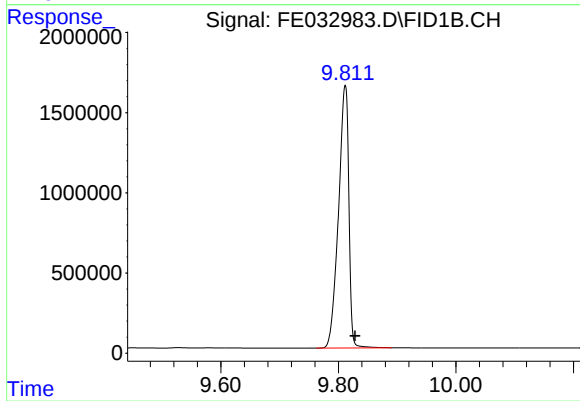


#5 N-HEXADECANE

R.T.: 9.812 min
Delta R.T.: -0.016 min
Response: 19997387
Conc: 56.37 ug/ml

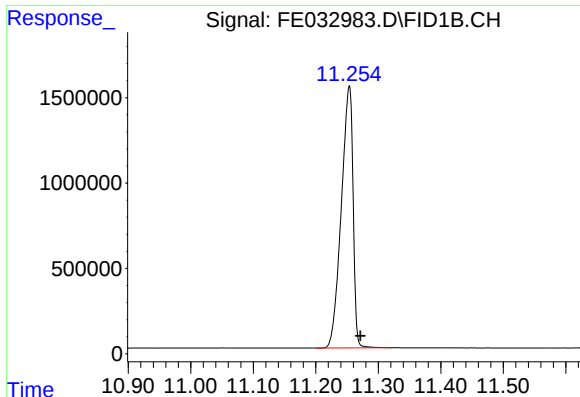


#6 N-OCTADECANE

R.T.: 11.254 min
Delta R.T.: -0.017 min
Response: 20060728
Conc: 55.63 ug/ml

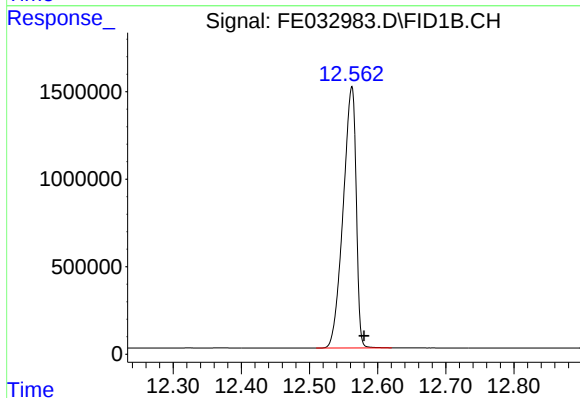


#7 N-EICOSANE

R.T.: 12.562 min
Delta R.T.: -0.018 min
Response: 19827017
Conc: 55.26 ug/ml

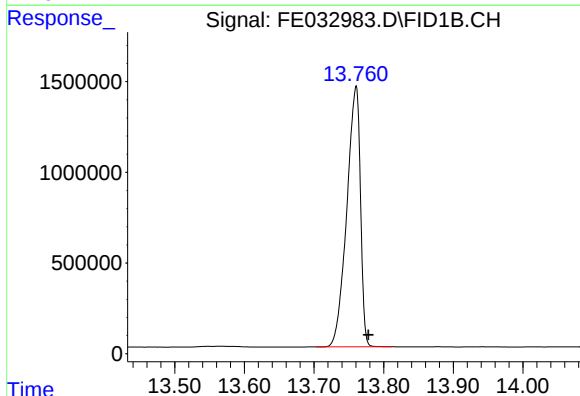


#8 N-DOCOSANE

R.T.: 13.761 min
Delta R.T.: -0.017 min
Response: 19517313
Conc: 54.87 ug/ml

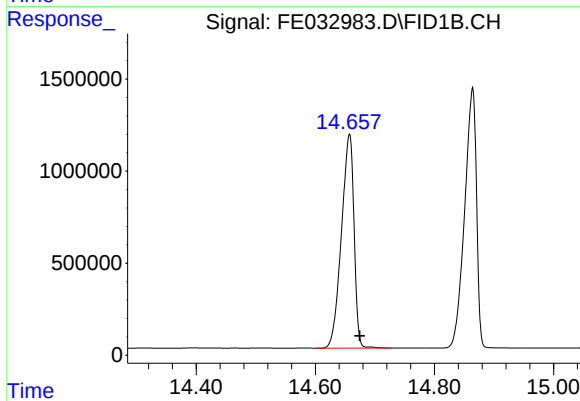


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.657 min
Delta R.T.: -0.017 min
Response: 17040679
Conc: 55.02 ug/ml

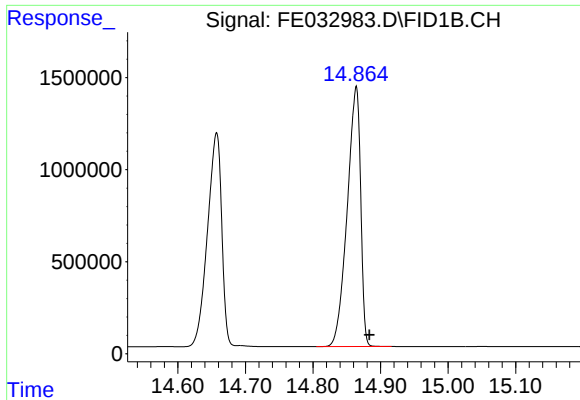


#10 N-TETRACOSANE

R.T.: 14.864 min
Delta R.T.: -0.020 min
Response: 19506449
Conc: 54.74 ug/ml

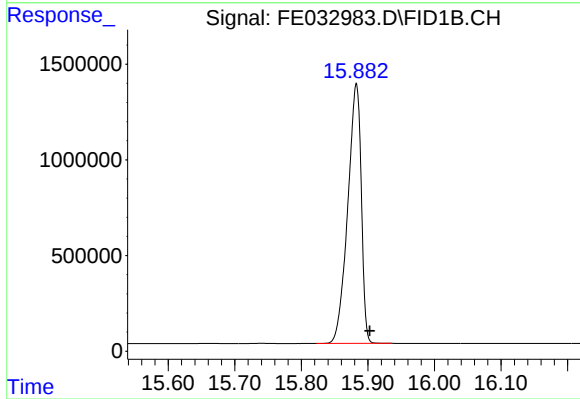

#11 N-HEXACOSANE

R.T.: 15.883 min
Delta R.T.: -0.020 min
Response: 19121190
Conc: 54.58 ug/ml

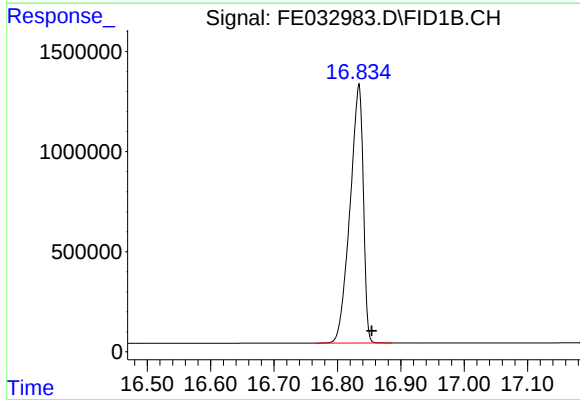

#12 N-OCTACOSANE

R.T.: 16.834 min
Delta R.T.: -0.020 min
Response: 18823268
Conc: 54.31 ug/ml