

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101723AL\
Data File : FE044883.D
Signal(s) : FID1B.ch
Acq On : 17 Oct 2023 07:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 17 10:46:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 101123.M
Quant Title : GC Extractables
QLast Update : Thu Oct 12 06:15:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.912	787225	5.245 ug/ml
20) T	n-Hexatriacontane (C36)	20.487	125531	0.817 ug/ml
21) T	n-Octatriacontane (C38)	21.118f	1005603	6.438 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101723AL\
Data File : FE044883.D
Signal(s) : FID1B.ch
Acq On : 17 Oct 2023 07:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 17 10:46:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 101123.M
Quant Title : GC Extractables
QLast Update : Thu Oct 12 06:15:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

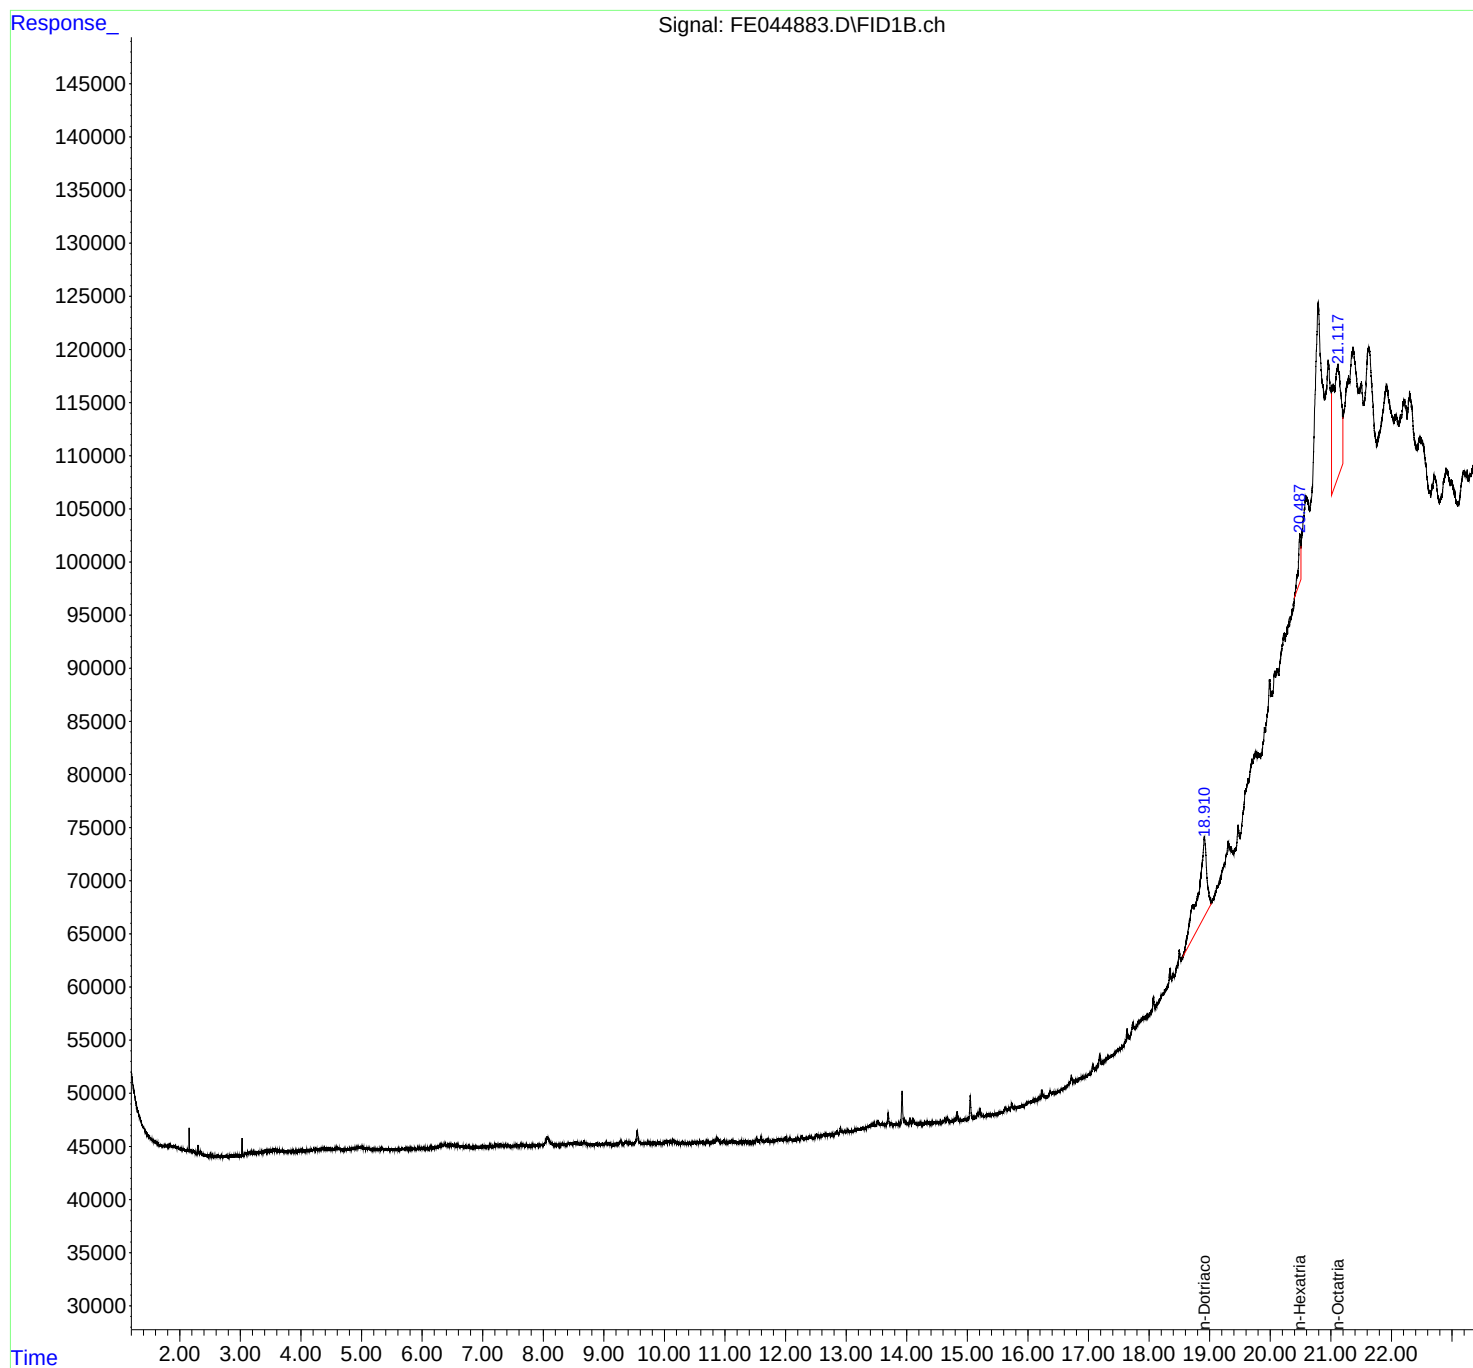


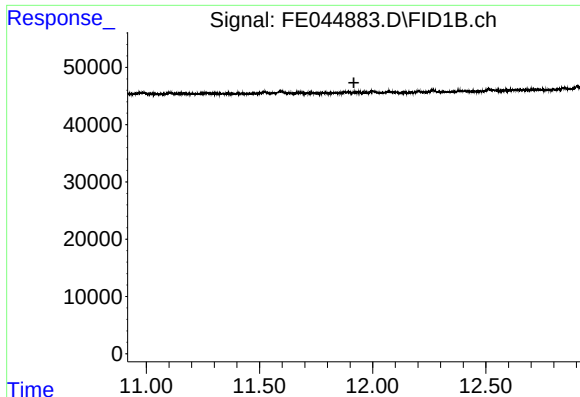

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.917 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

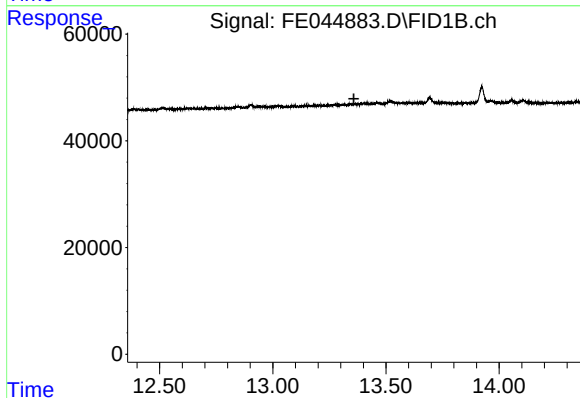


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.358 min
Response: 0
Conc: N.D.

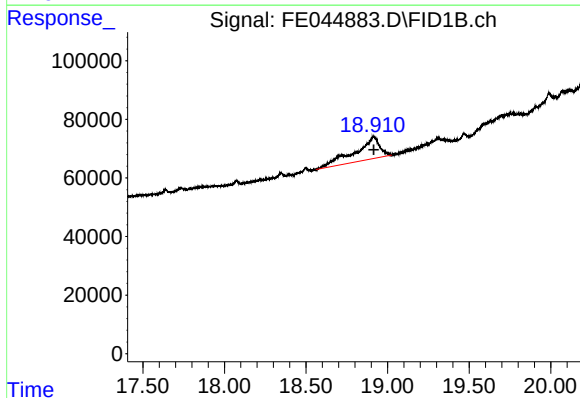


#18 n-Dotriacontane (C32)

R.T.: 18.912 min
Delta R.T.: -0.004 min
Response: 787225
Conc: 5.24 ug/ml

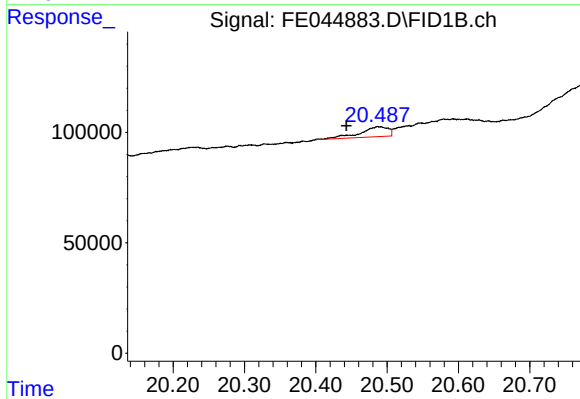

#20 n-Hexatriacontane (C36)

R.T.: 20.487 min
Delta R.T.: 0.044 min
Response: 125531
Conc: 0.82 ug/ml

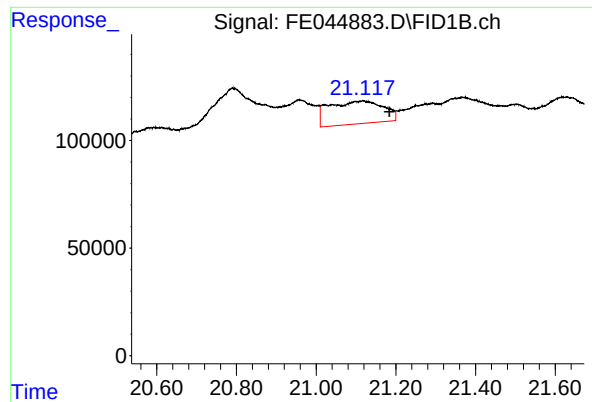

#21 n-Octatriacontane (C38)

R.T.: 21.118 min
Delta R.T.: -0.066 min
Response: 1005603
Conc: 6.44 ug/ml

Instrument :

FID_E

ClientSampleId :