

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101923AL\
Data File : FE044940.D
Signal(s) : FID1B.ch
Acq On : 20 Oct 2023 00:29
Operator : YP\AJ
Sample : 04843-02DL 500X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 20 01:18:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 101223.M
Quant Title : GC Extractables
QLast Update : Thu Oct 12 06:15:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.916	151209	1.007 ug/ml
20) T	n-Hexatriacontane (C36)	20.471	209173	1.361 ug/ml
22) T	n-Tetracontane (C40)	22.131	244896	1.465 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE101923AL\
Data File : FE044940.D
Signal(s) : FID1B.ch
Acq On : 20 Oct 2023 00:29
Operator : YP\AJ
Sample : 04843-02DL 500X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 20 01:18:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 101223.M
Quant Title : GC Extractables
QLast Update : Thu Oct 12 06:15:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

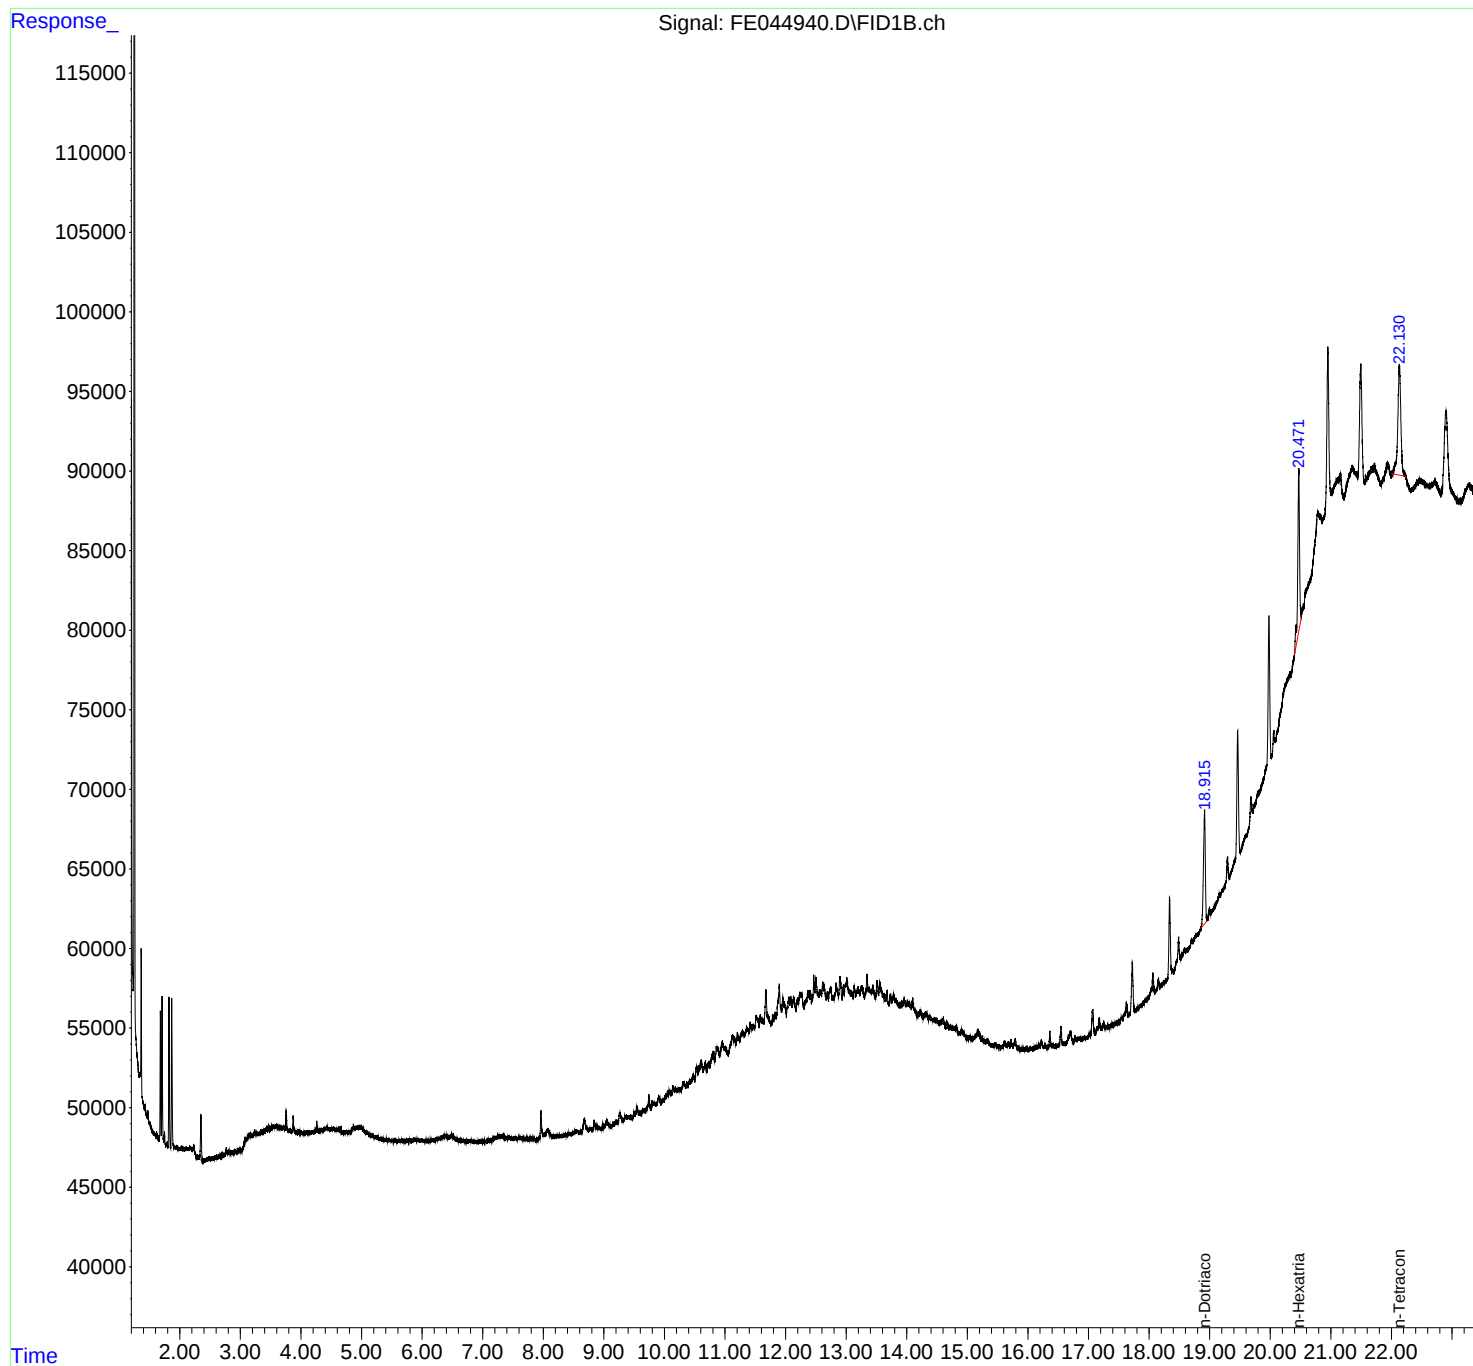


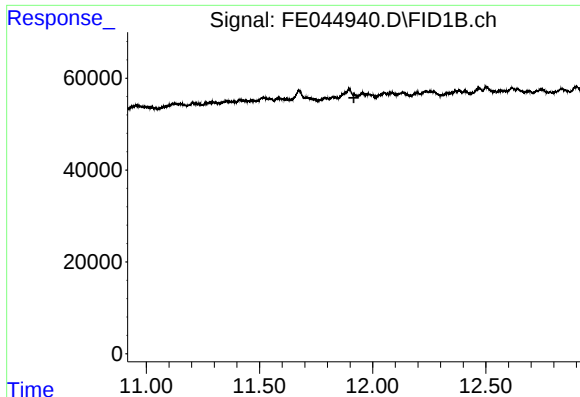

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.917 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

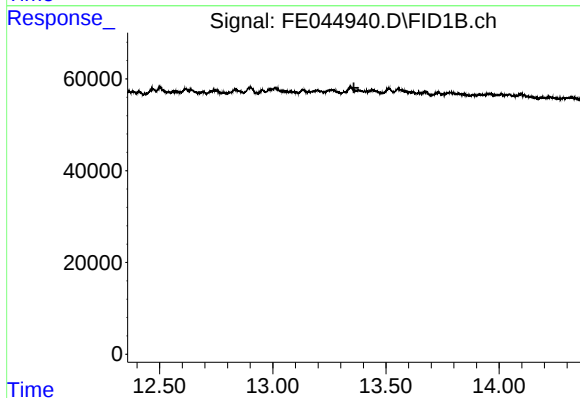


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.358 min
Response: 0
Conc: N.D.

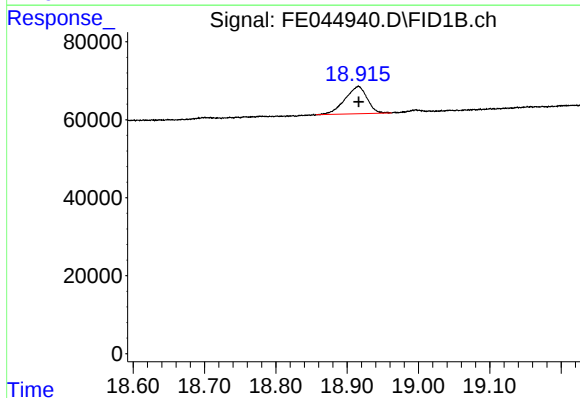


#18 n-Dotriacontane (C32)

R.T.: 18.916 min
Delta R.T.: 0.000 min
Response: 151209
Conc: 1.01 ug/ml

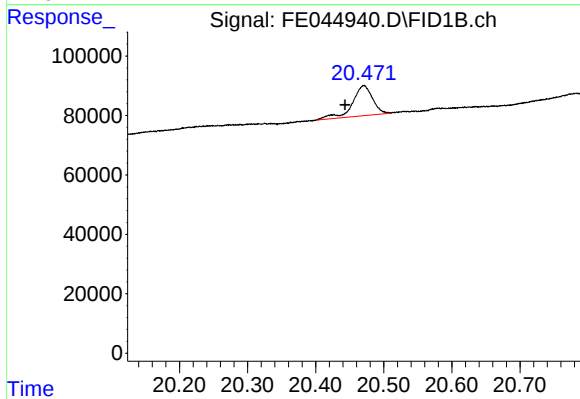

#20 n-Hexatriacontane (C36)

R.T.: 20.471 min
Delta R.T.: 0.028 min
Response: 209173
Conc: 1.36 ug/ml

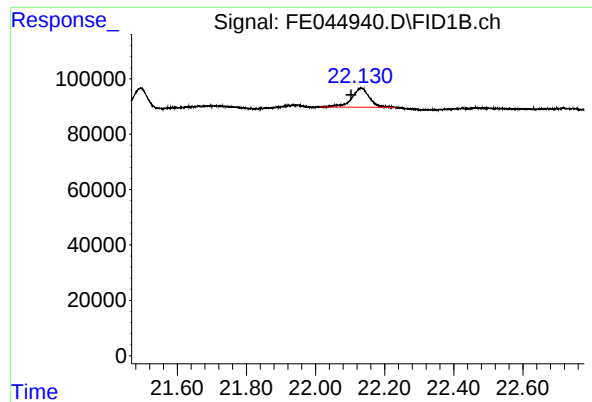

#22 n-Tetracontane (C40)

R.T.: 22.131 min
Delta R.T.: 0.028 min
Response: 244896
Conc: 1.47 ug/ml

Instrument :

FID_E

ClientSampleId :