

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102022AL\
Data File : FE038250.D
Signal(s) : FID1B.ch
Acq On : 20 Oct 2022 23:39
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 21 04:07:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 092822.M
Quant Title : GC Extractables
QLast Update : Wed Sep 28 06:23:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.544	44578	0.283 ug/ml
21) T	n-Octatriacontane (C38)	20.802	1958323	14.431 ug/ml
22) T	n-Tetracontane (C40)	21.475	912849	7.171 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102022AL\
Data File : FE038250.D
Signal(s) : FID1B.ch
Acq On : 20 Oct 2022 23:39
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 21 04:07:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 092822.M
Quant Title : GC Extractables
QLast Update : Wed Sep 28 06:23:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

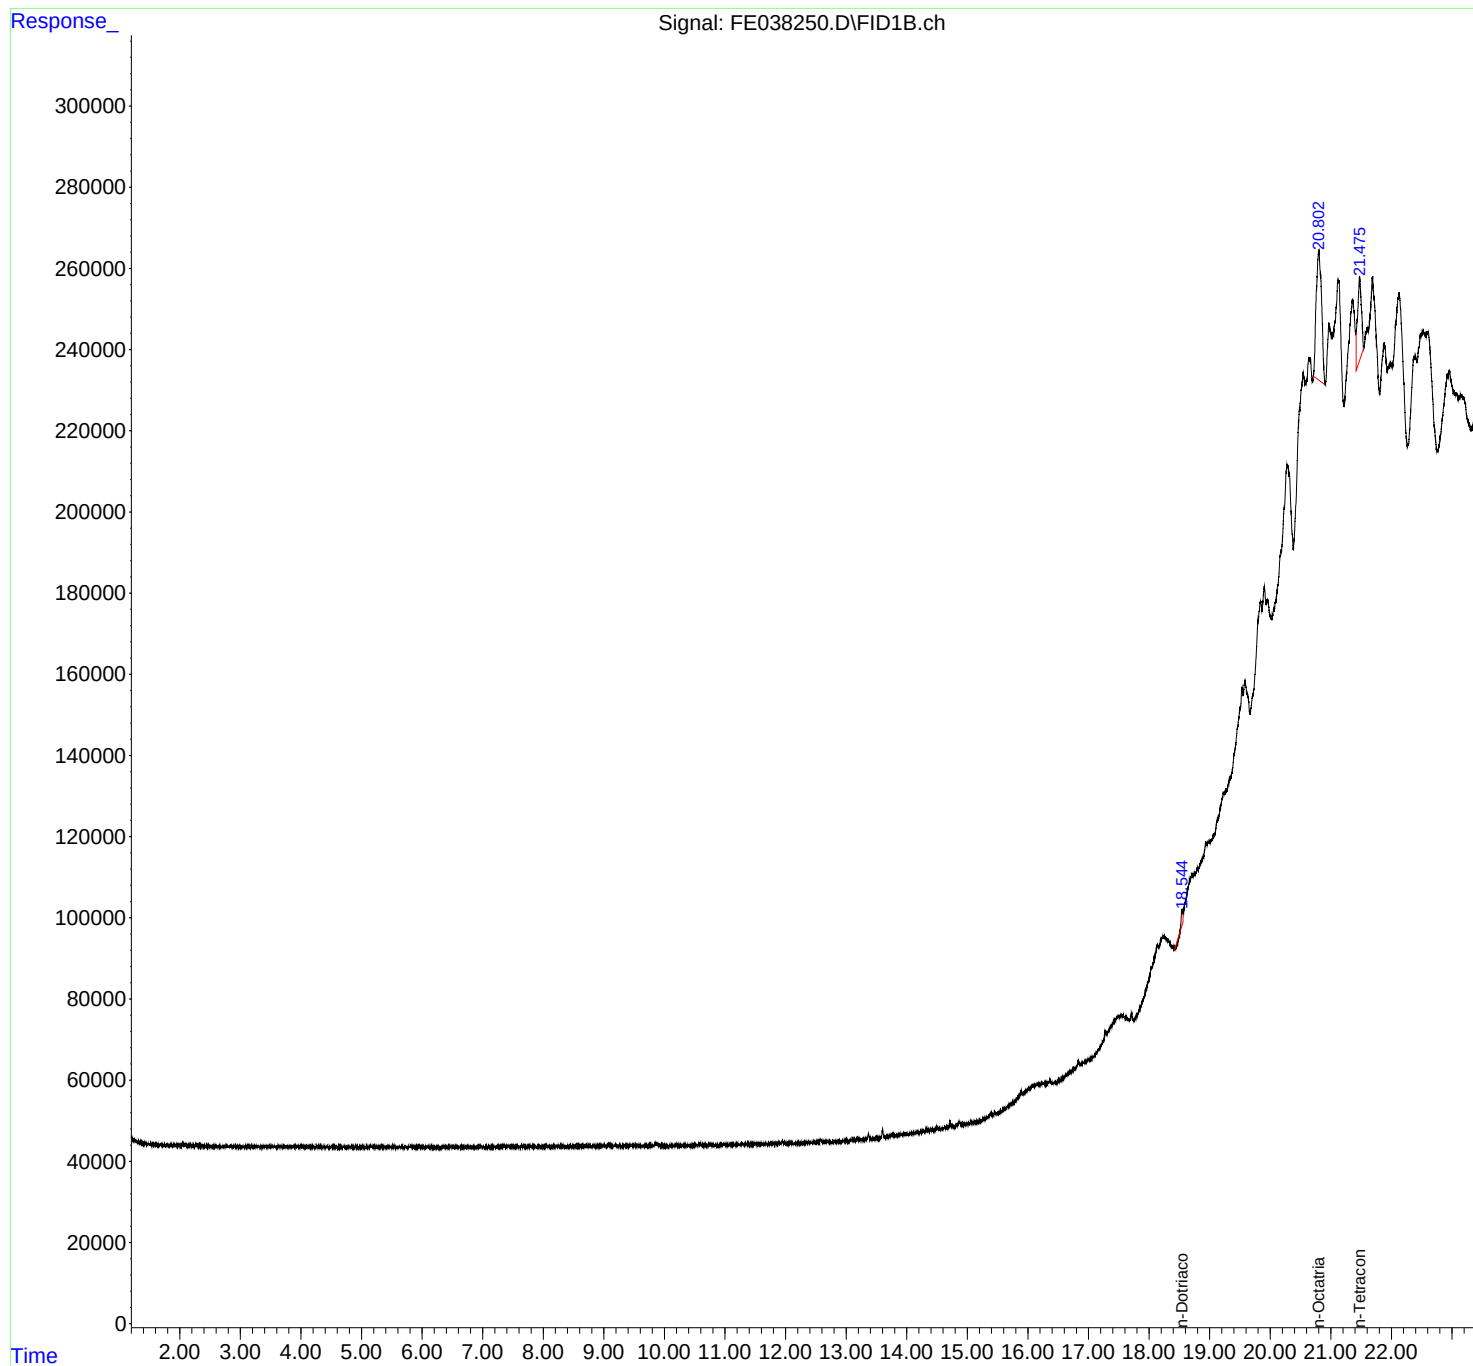


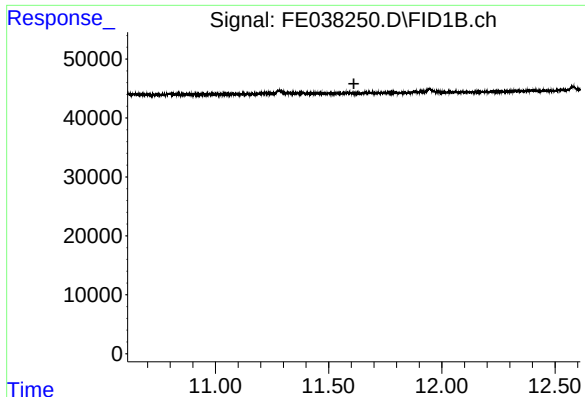

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.612 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

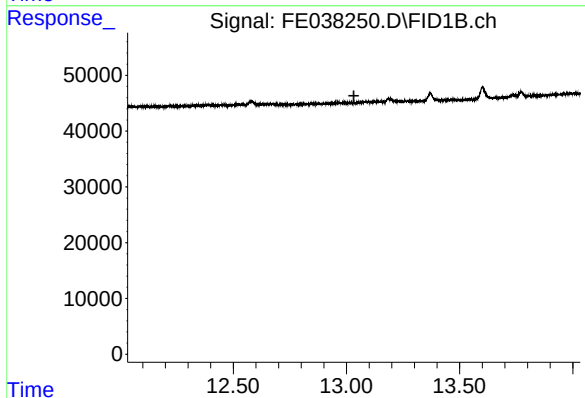


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.033 min
Response: 0
Conc: N.D.

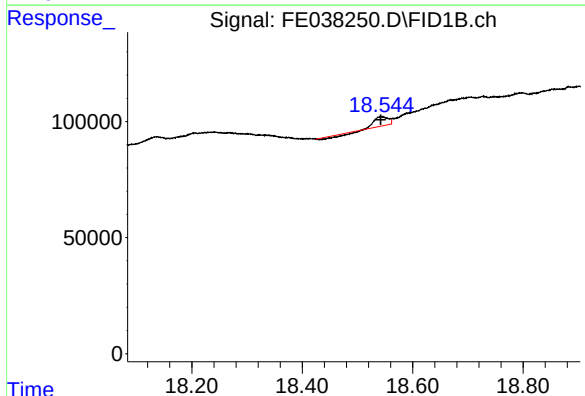


#18 n-Dotriacontane (C32)

R.T.: 18.544 min
Delta R.T.: 0.002 min
Response: 44578
Conc: 0.28 ug/ml

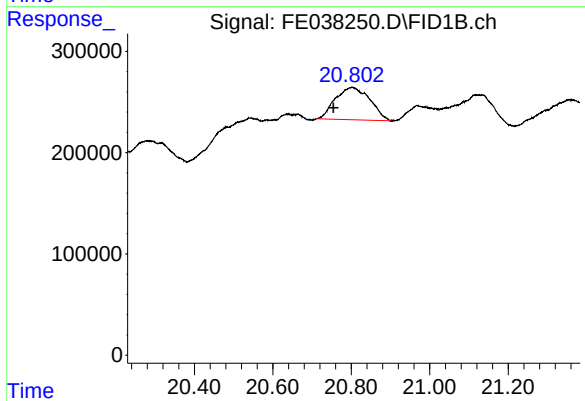

#21 n-Octatriacontane (C38)

R.T.: 20.802 min
Delta R.T.: 0.047 min
Response: 1958323
Conc: 14.43 ug/ml

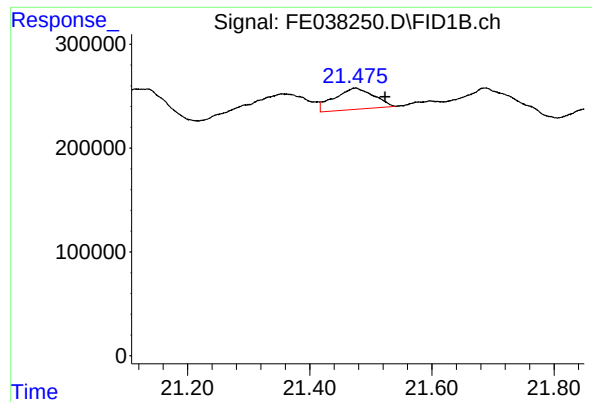

#22 n-Tetracontane (C40)

R.T.: 21.475 min
Delta R.T.: -0.048 min
Response: 912849
Conc: 7.17 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK