

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102120\
Data File : FE033022.D
Signal(s) : FID1B.CH
Acq On : 21 Oct 2020 8:53
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 22 00:56:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101420.M
Quant Title :
QLast Update : Wed Oct 14 02:47:05 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.546	206008	0.636 ug/ml
16)	N-HEXATRIACONTANE	20.099	387547	1.529 ug/ml
18)	N-TETRACONTANE	21.750	704898	3.227 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102120\
Data File : FE033022.D
Signal(s) : FID1B.CH
Acq On : 21 Oct 2020 8:53
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 22 00:56:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101420.M
Quant Title :
QLast Update : Wed Oct 14 02:47:05 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

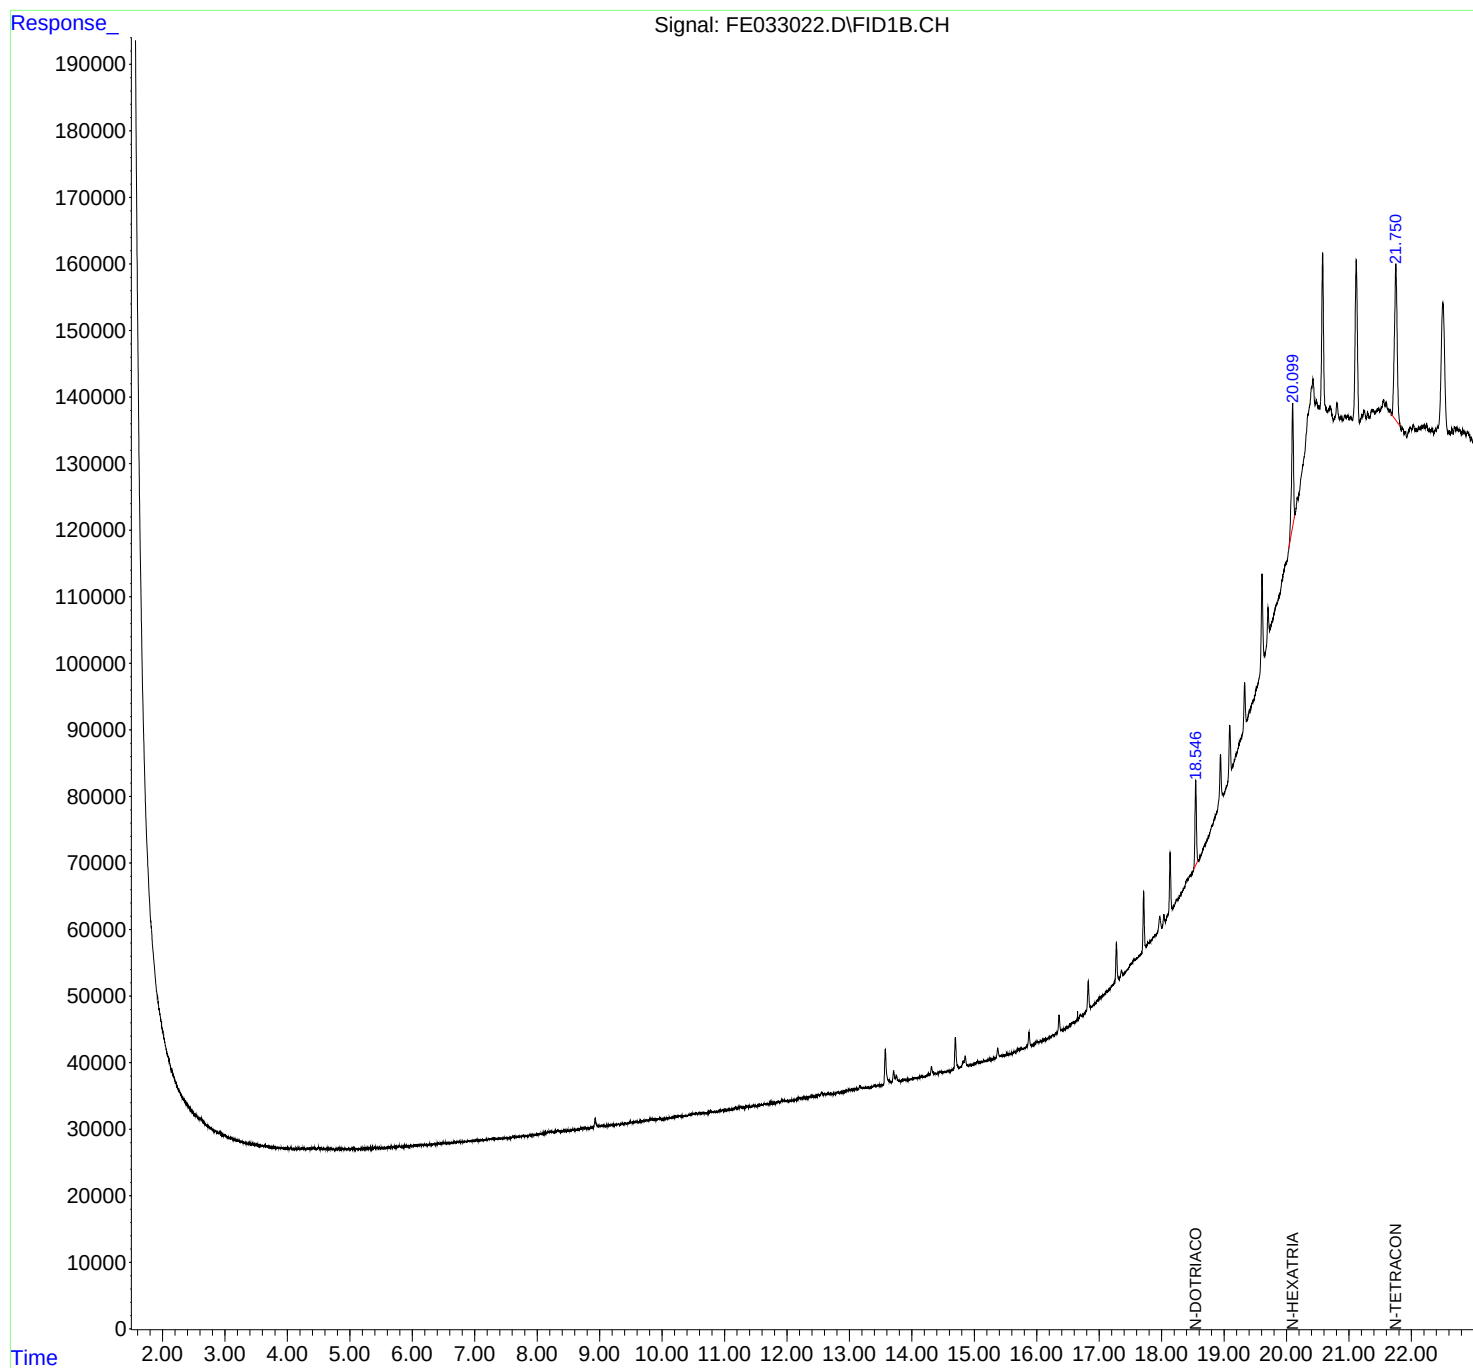


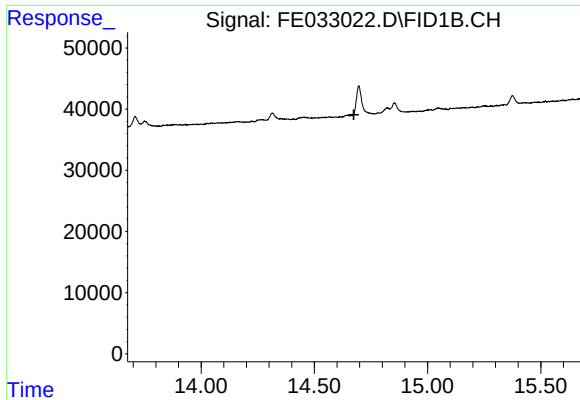

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.674 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

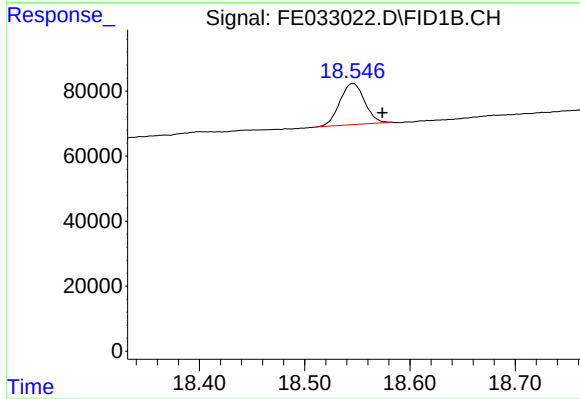


#14 N-DOTRIACONTANE

R.T.: 18.546 min
Delta R.T.: -0.028 min
Response: 206008
Conc: 0.64 ug/ml

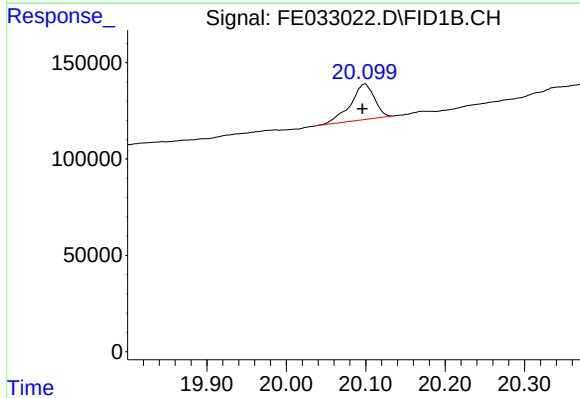

#16 N-HEXATRIACONTANE

R.T.: 20.099 min
Delta R.T.: 0.003 min
Response: 387547
Conc: 1.53 ug/ml

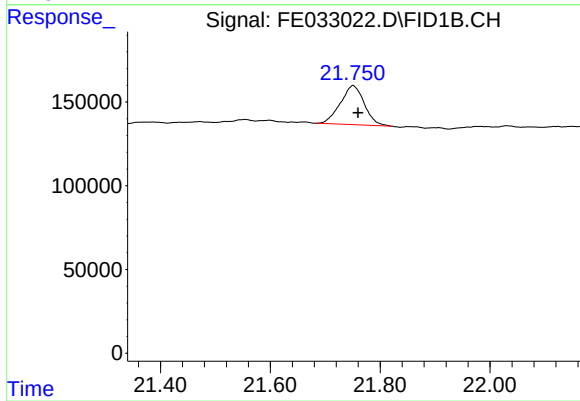

#18 N-TETRACONTANE

R.T.: 21.750 min
Delta R.T.: -0.009 min
Response: 704898
Conc: 3.23 ug/ml