

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102120\
 Data File : FE033031.D
 Signal(s) : FID1B.CH
 Acq On : 21 Oct 2020 15:48
 Operator : DD\AJ
 Sample : L4436-11 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 22 00:58:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101420.M
 Quant Title :
 QLast Update : Wed Oct 14 02:47:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	319436	1.031 ug/ml
Target Compounds			
7) N-EICOSANE	12.632f	1860302	5.185 ug/ml
10) N-TETRACOSANE	14.861	893177	2.506 ug/ml
12) N-OCTACOSANE	16.823	150189	0.433 ug/ml
13) N-TRIACONTANE	17.714	455022	1.330 ug/ml
14) N-DOTRIACONTANE	18.546	642816	1.986 ug/ml
15) N-TETRATRIACONTANE	19.331	212849	0.729 ug/ml
16) N-HEXATRIACONTANE	20.103	1700951	6.710 ug/ml
18) N-TETRACONTANE	21.759	1048907	4.802 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102120\
Data File : FE033031.D
Signal(s) : FID1B.CH
Acq On : 21 Oct 2020 15:48
Operator : DD\AJ
Sample : L4436-11 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 22 00:58:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE101420.M
Quant Title :
QLast Update : Wed Oct 14 02:47:05 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

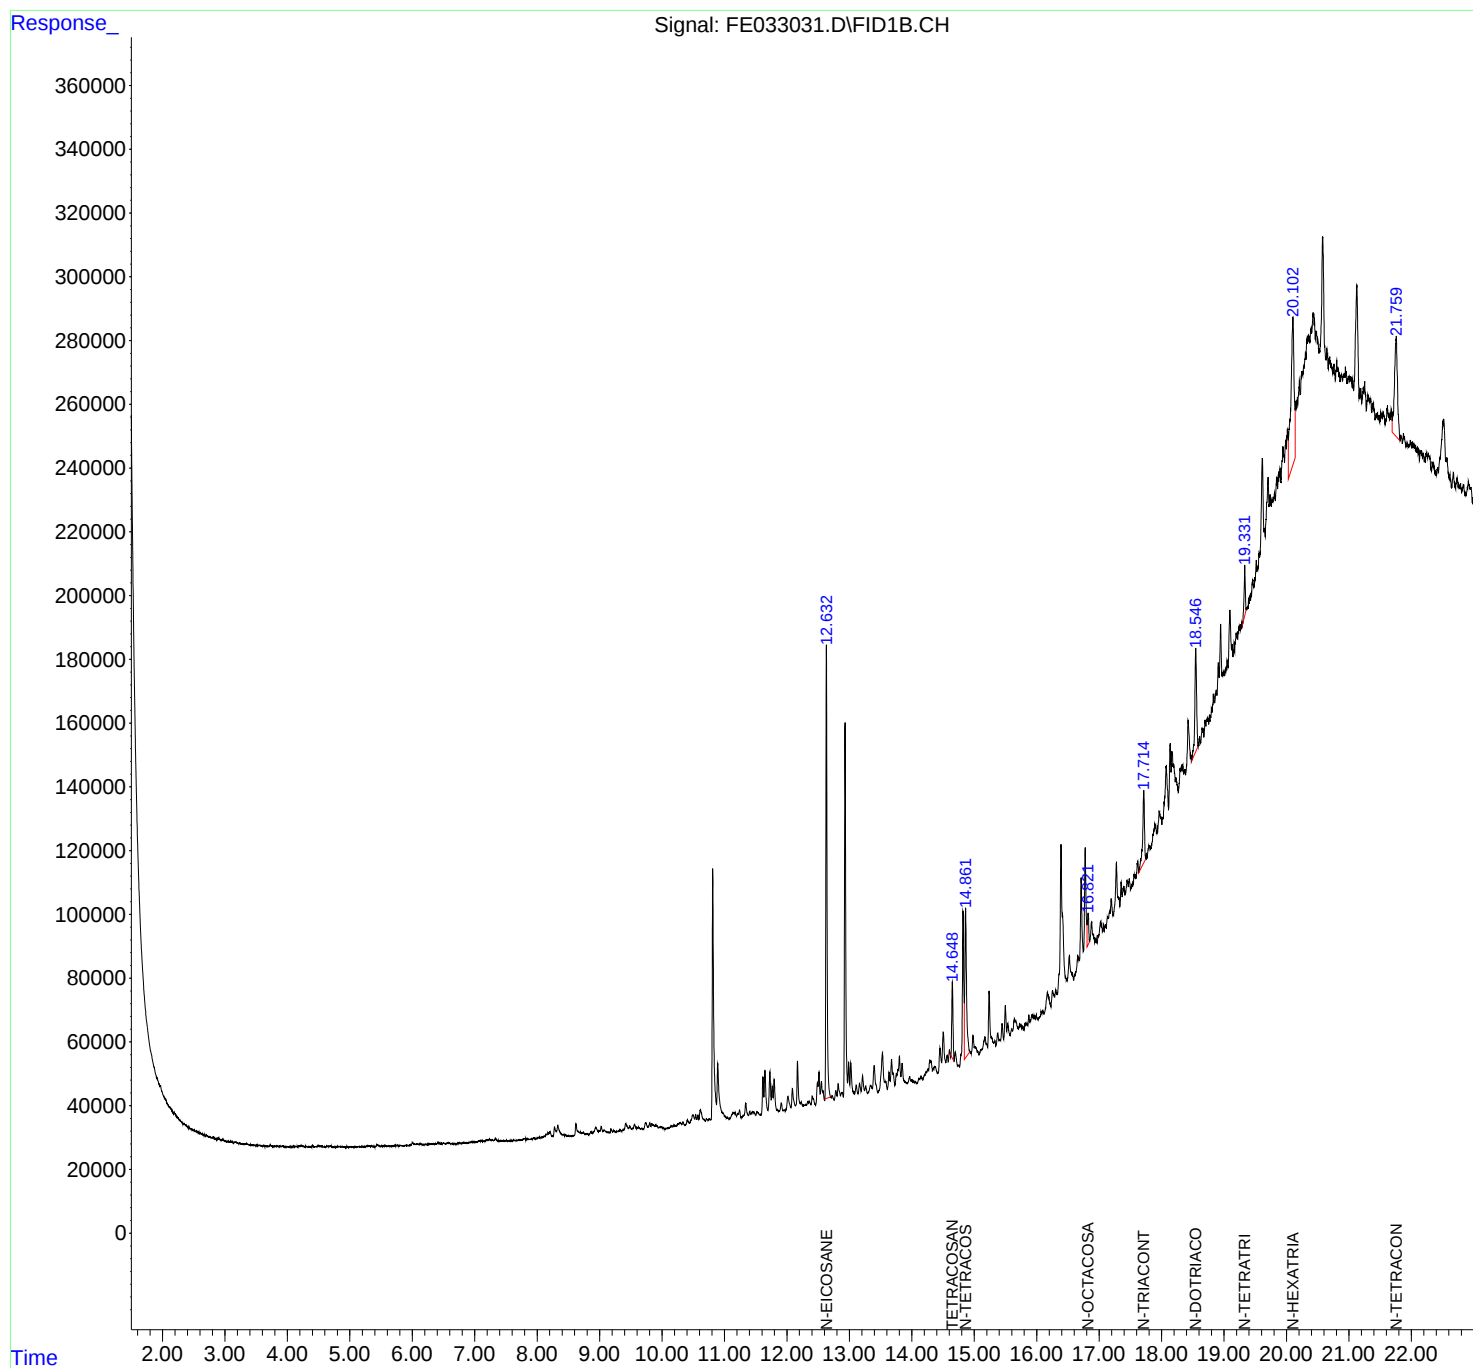


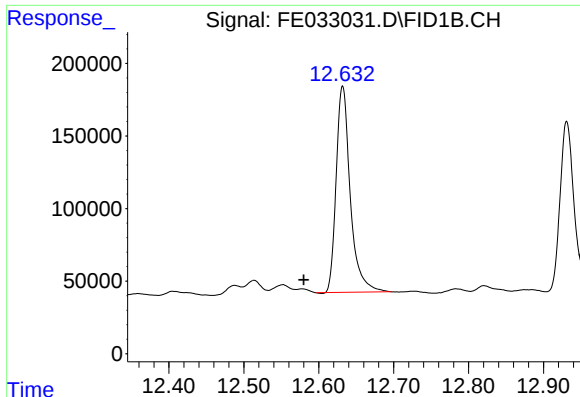

#7 N-EICOSANE


R.T.: 12.632 min
Delta R.T.: 0.052 min
Response: 1860302
Conc: 5.18 ug/ml

Instrument :
FID_E
ClientSampleId :

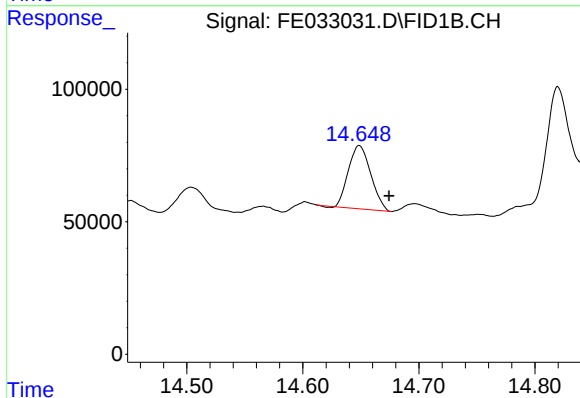


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.649 min
Delta R.T.: -0.026 min
Response: 319436
Conc: 1.03 ug/ml

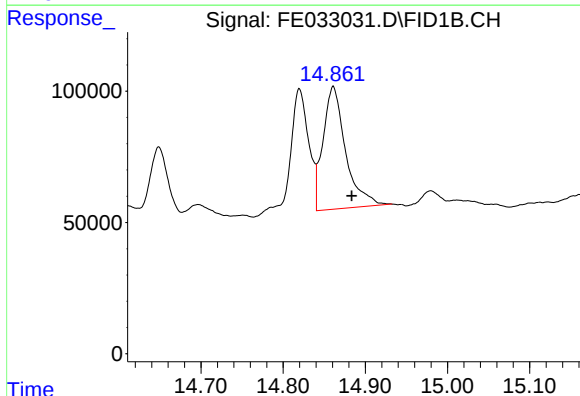


#10 N-TETRACOSANE

R.T.: 14.861 min
Delta R.T.: -0.023 min
Response: 893177
Conc: 2.51 ug/ml

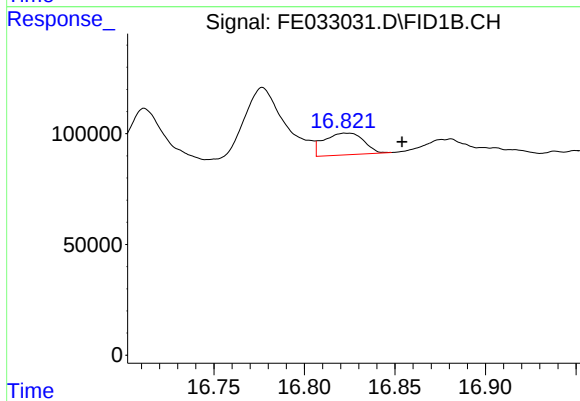

#12 N-OCTACOSANE


R.T.: 16.823 min
Delta R.T.: -0.031 min
Response: 150189
Conc: 0.43 ug/ml

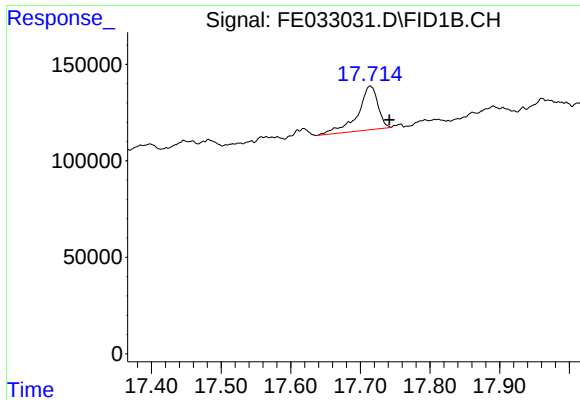

#13 N-TRIACONTANE


R.T.: 17.714 min
Delta R.T.: -0.028 min
Response: 455022
Conc: 1.33 ug/ml

Instrument :
FID_E
ClientSampleId :

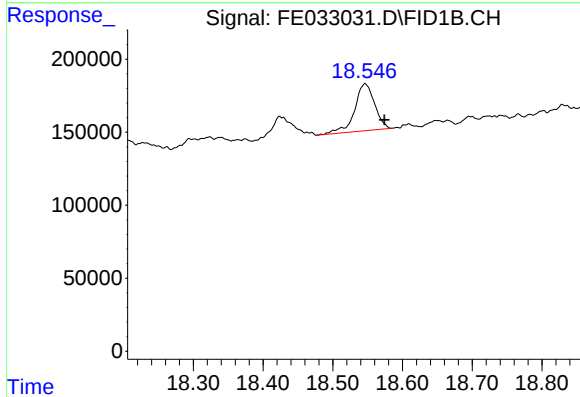


#14 N-DOTRIACONTANE

R.T.: 18.546 min
Delta R.T.: -0.028 min
Response: 642816
Conc: 1.99 ug/ml

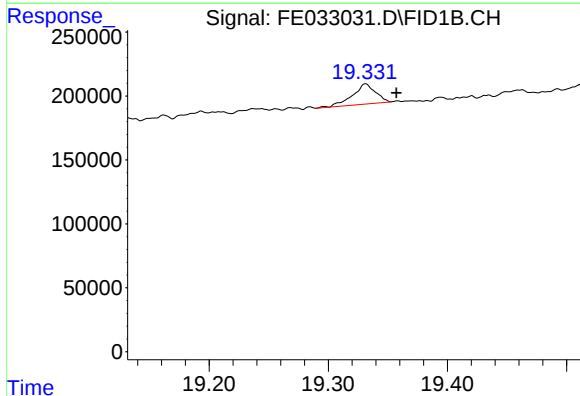


#15 N-TETRATRIACONTANE

R.T.: 19.331 min
Delta R.T.: -0.026 min
Response: 212849
Conc: 0.73 ug/ml

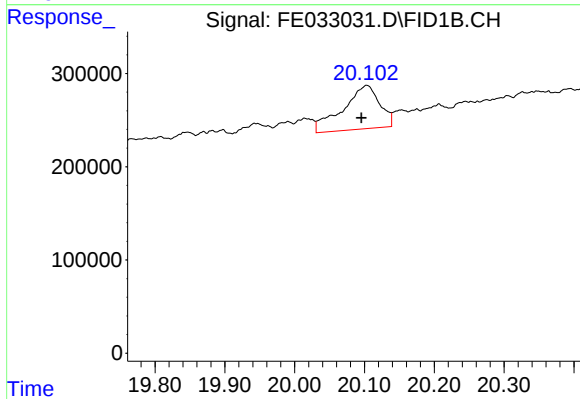

#16 N-HEXATRIACONTANE

R.T.: 20.103 min
Delta R.T.: 0.008 min
Response: 1700951
Conc: 6.71 ug/ml

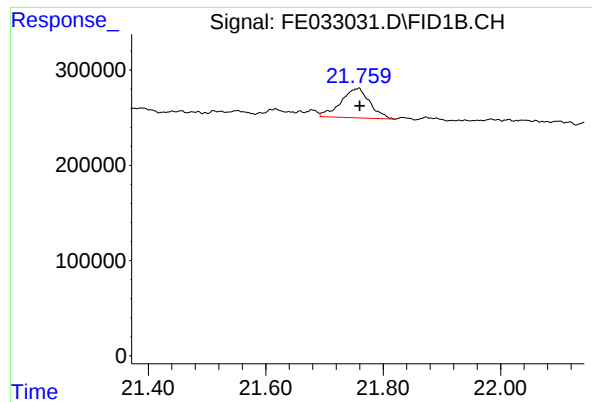

#18 N-TETRACONTANE

R.T.: 21.759 min
Delta R.T.: 0.000 min
Response: 1048907
Conc: 4.80 ug/ml

Instrument :
FID_E
ClientSampleId :