

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102122AL\
 Data File : FE038252.D
 Signal(s) : FID1B.ch
 Acq On : 21 Oct 2022 08:17
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 21 11:14:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 092822.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 28 06:23:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.558	221227	1.357 ug/ml
11) T	n-Heneicosane (C21)	13.177	207398	1.259 ug/ml
13) T	n-Docosane (C22)	13.763	143606	0.872 ug/ml
14) T	n-Tetracosane (C24)	14.862	168177	1.025 ug/ml
15) T	n-Hexacosane (C26)	15.880	123789	0.759 ug/ml
16) T	n-Octacosane (C28)	16.827	91481	0.571 ug/ml
17) T	n-Tricontane (C30)	17.711	107731	0.673 ug/ml
18) T	n-Dotriacontane (C32)	18.537	230287	1.462 ug/ml
20) T	n-Hexatriacontane (C36)	20.058	41526	0.288 ug/ml
21) T	n-Octatriacontane (C38)	20.750	96766	0.713 ug/ml
22) T	n-Tetracontane (C40)	21.475	806879	6.339 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102122AL\
Data File : FE038252.D
Signal(s) : FID1B.ch
Acq On : 21 Oct 2022 08:17
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 21 11:14:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 092822.M
Quant Title : GC Extractables
QLast Update : Wed Sep 28 06:23:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

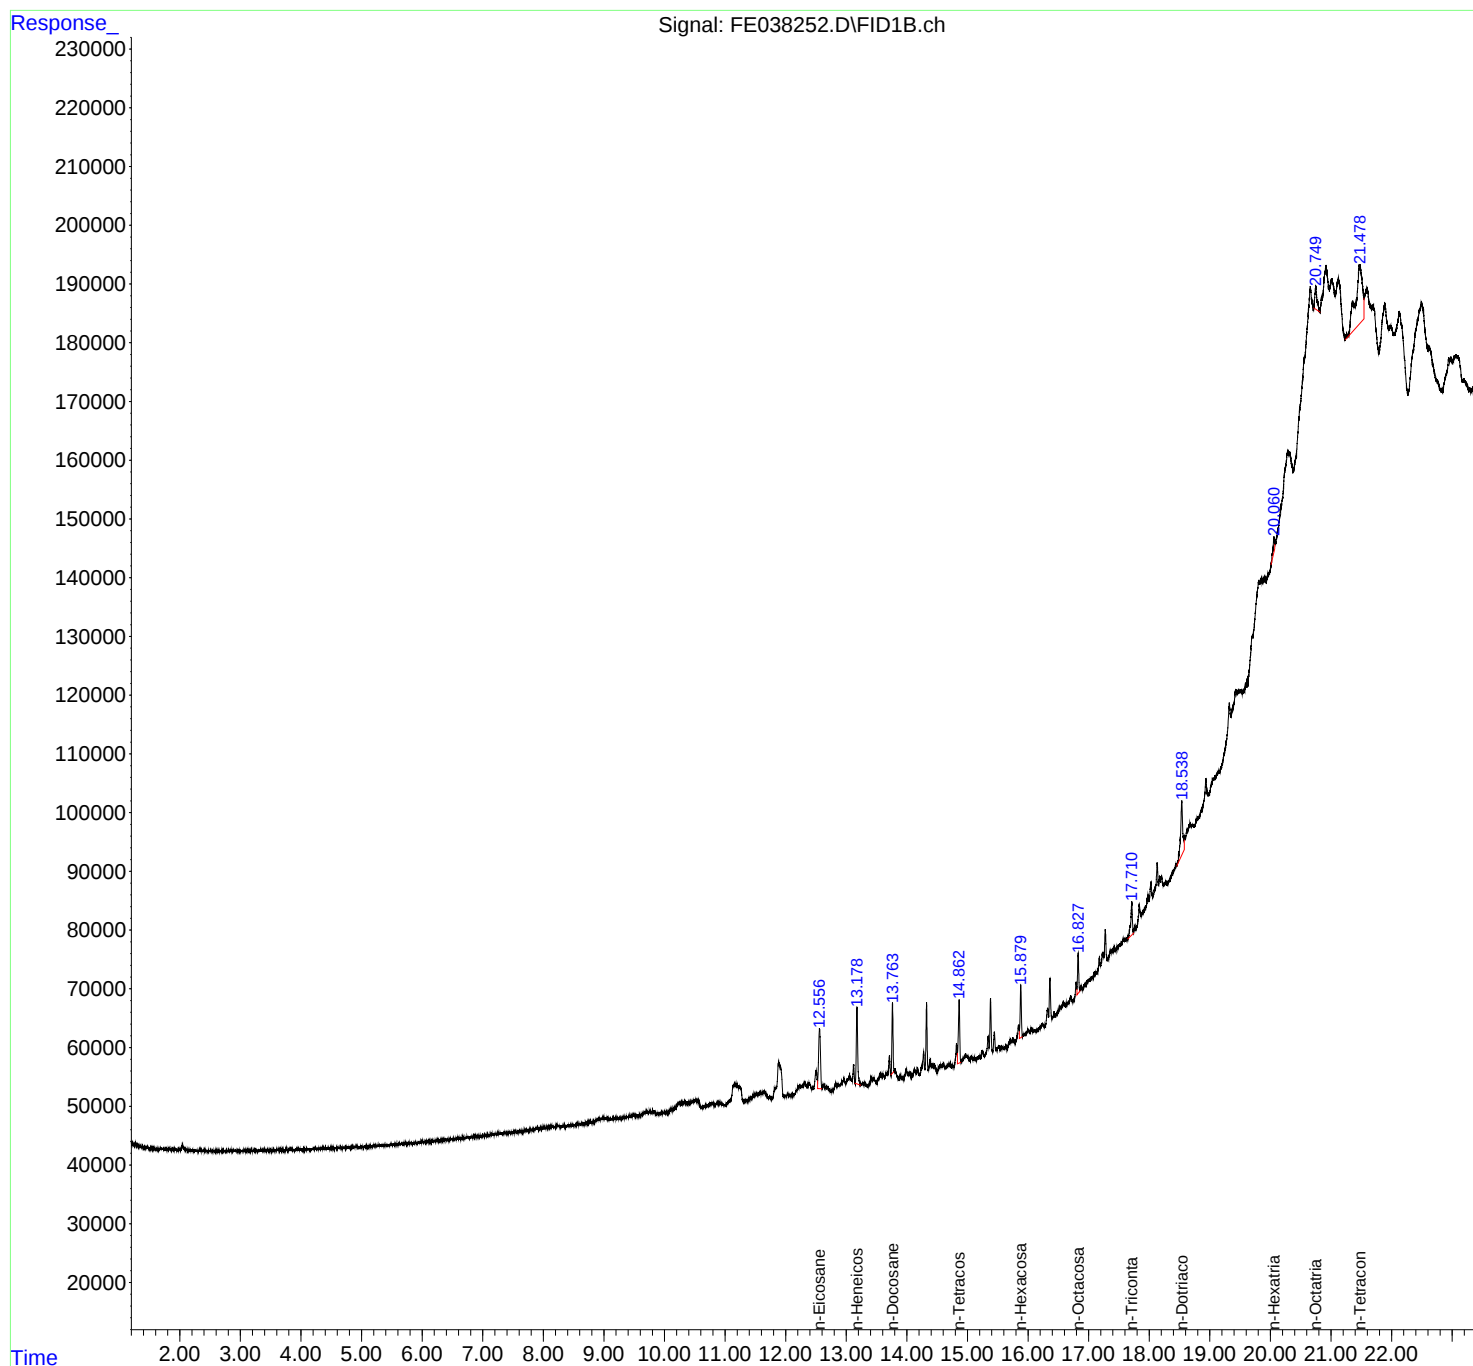


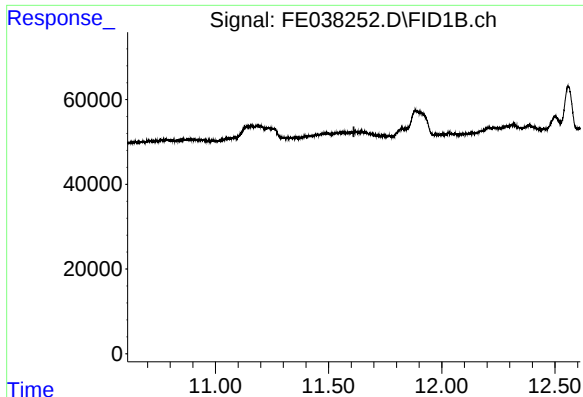

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.612 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

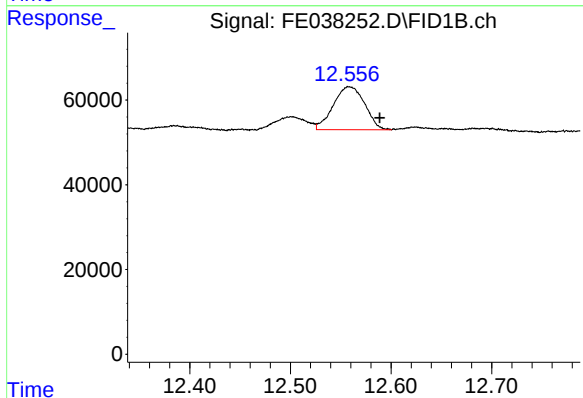


#10 n-Eicosane (C20)

R.T.: 12.558 min
Delta R.T.: -0.030 min
Response: 221227
Conc: 1.36 ug/ml

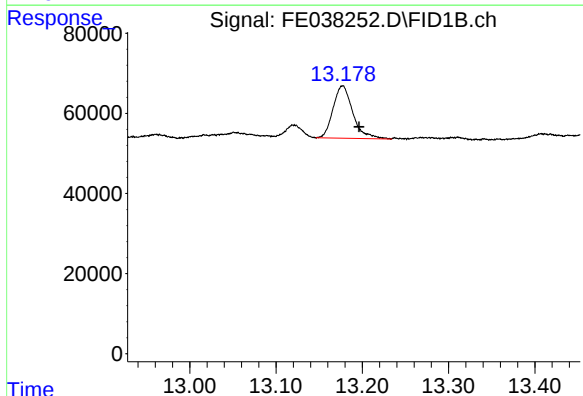


#11 n-Heneicosane (C21)

R.T.: 13.177 min
Delta R.T.: -0.019 min
Response: 207398
Conc: 1.26 ug/ml

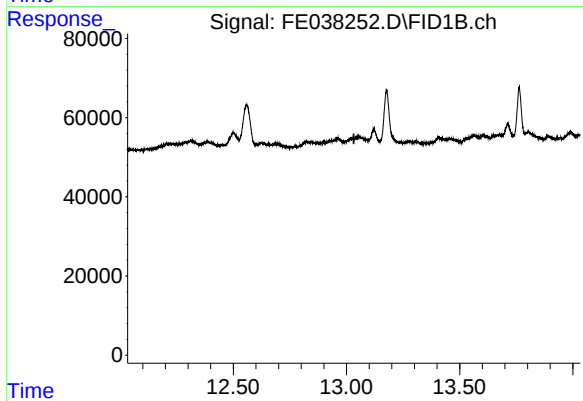

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.033 min
Response: 0
Conc: N.D.

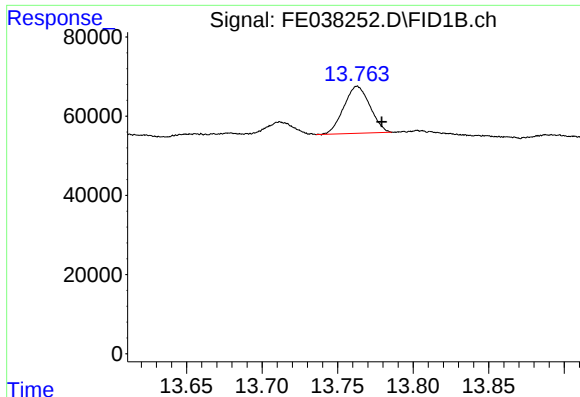

#13 n-Docosane (C22)


R.T.: 13.763 min
Delta R.T.: -0.016 min
Response: 143606
Conc: 0.87 ug/ml

Instrument :
FID_E
ClientSampleId :

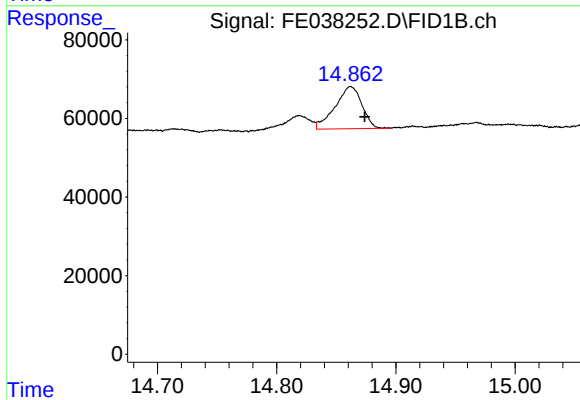


#14 n-Tetracosane (C24)

R.T.: 14.862 min
Delta R.T.: -0.012 min
Response: 168177
Conc: 1.03 ug/ml

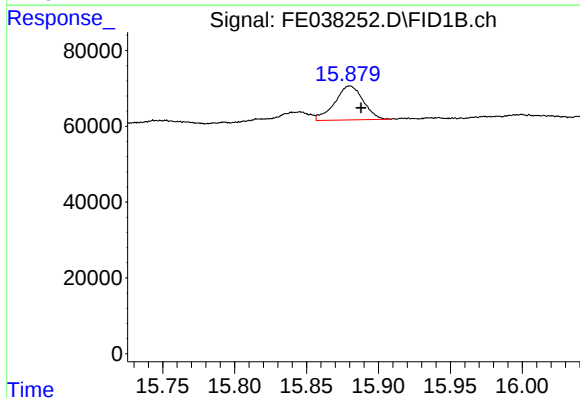


#15 n-Hexacosane (C26)

R.T.: 15.880 min
Delta R.T.: -0.008 min
Response: 123789
Conc: 0.76 ug/ml

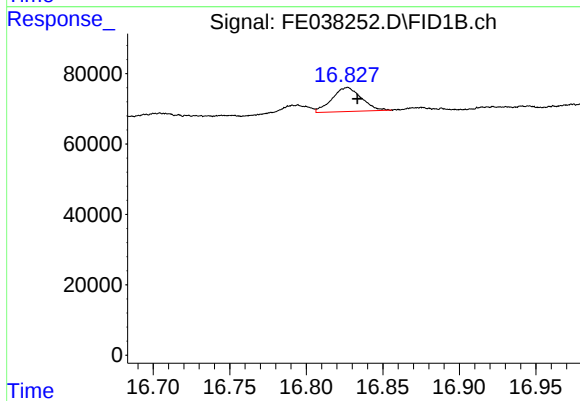

#16 n-Octacosane (C28)


R.T.: 16.827 min
Delta R.T.: -0.007 min
Response: 91481
Conc: 0.57 ug/ml

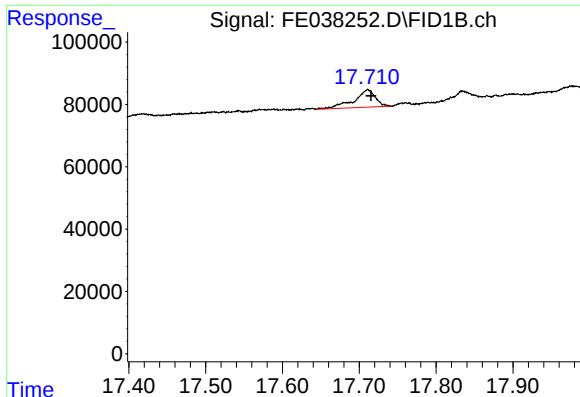

#17 n-Tricontane (C30)


R.T.: 17.711 min
Delta R.T.: -0.004 min
Response: 107731
Conc: 0.67 ug/ml

Instrument :
FID_E
ClientSampleId :

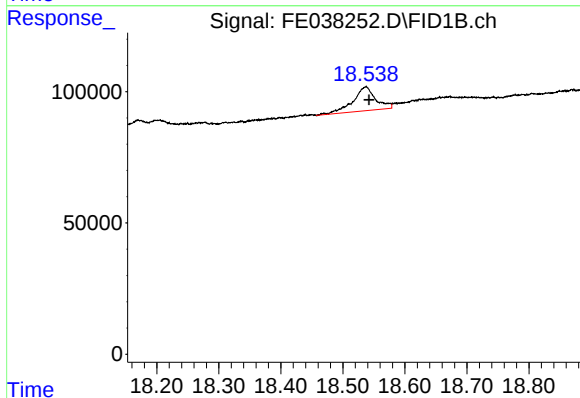


#18 n-Dotriacontane (C32)

R.T.: 18.537 min
Delta R.T.: -0.005 min
Response: 230287
Conc: 1.46 ug/ml

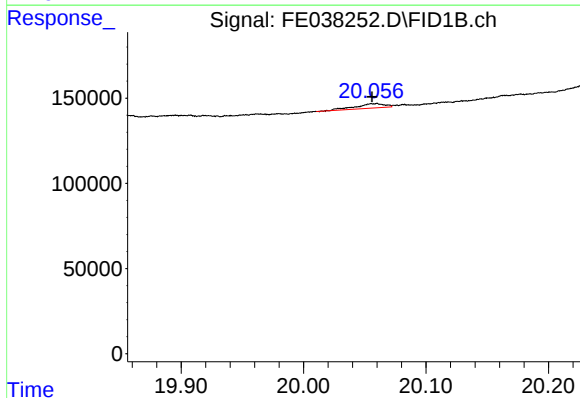


#20 n-Hexatriacontane (C36)

R.T.: 20.058 min
Delta R.T.: 0.002 min
Response: 41526
Conc: 0.29 ug/ml

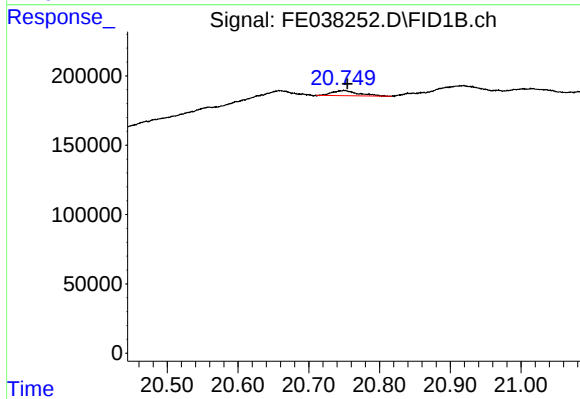

#21 n-Octatriacontane (C38)

R.T.: 20.750 min
Delta R.T.: -0.005 min
Response: 96766
Conc: 0.71 ug/ml

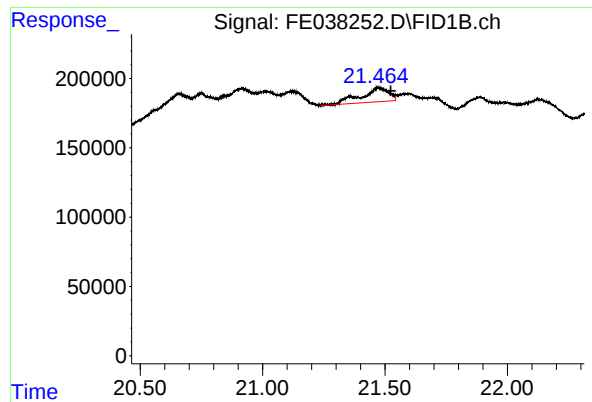

#22 n-Tetracontane (C40)

R.T.: 21.475 min
Delta R.T.: -0.048 min
Response: 806879
Conc: 6.34 ug/ml

Instrument :

FID_E

ClientSampleId :