

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102124AL\
 Data File : FE050736.D
 Signal(s) : FID1B.ch
 Acq On : 21 Oct 2024 11:49
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 22 04:46:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 100824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 07 16:32:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	18.011	61980	0.390 ug/ml
20) T n-Hexatriacontane (C36)	20.369	129981	1.025 ug/ml
22) T n-Tetracontane (C40)	21.986	273524	2.456 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102124AL\
Data File : FE050736.D
Signal(s) : FID1B.ch
Acq On : 21 Oct 2024 11:49
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 22 04:46:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 100824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 07 16:32:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

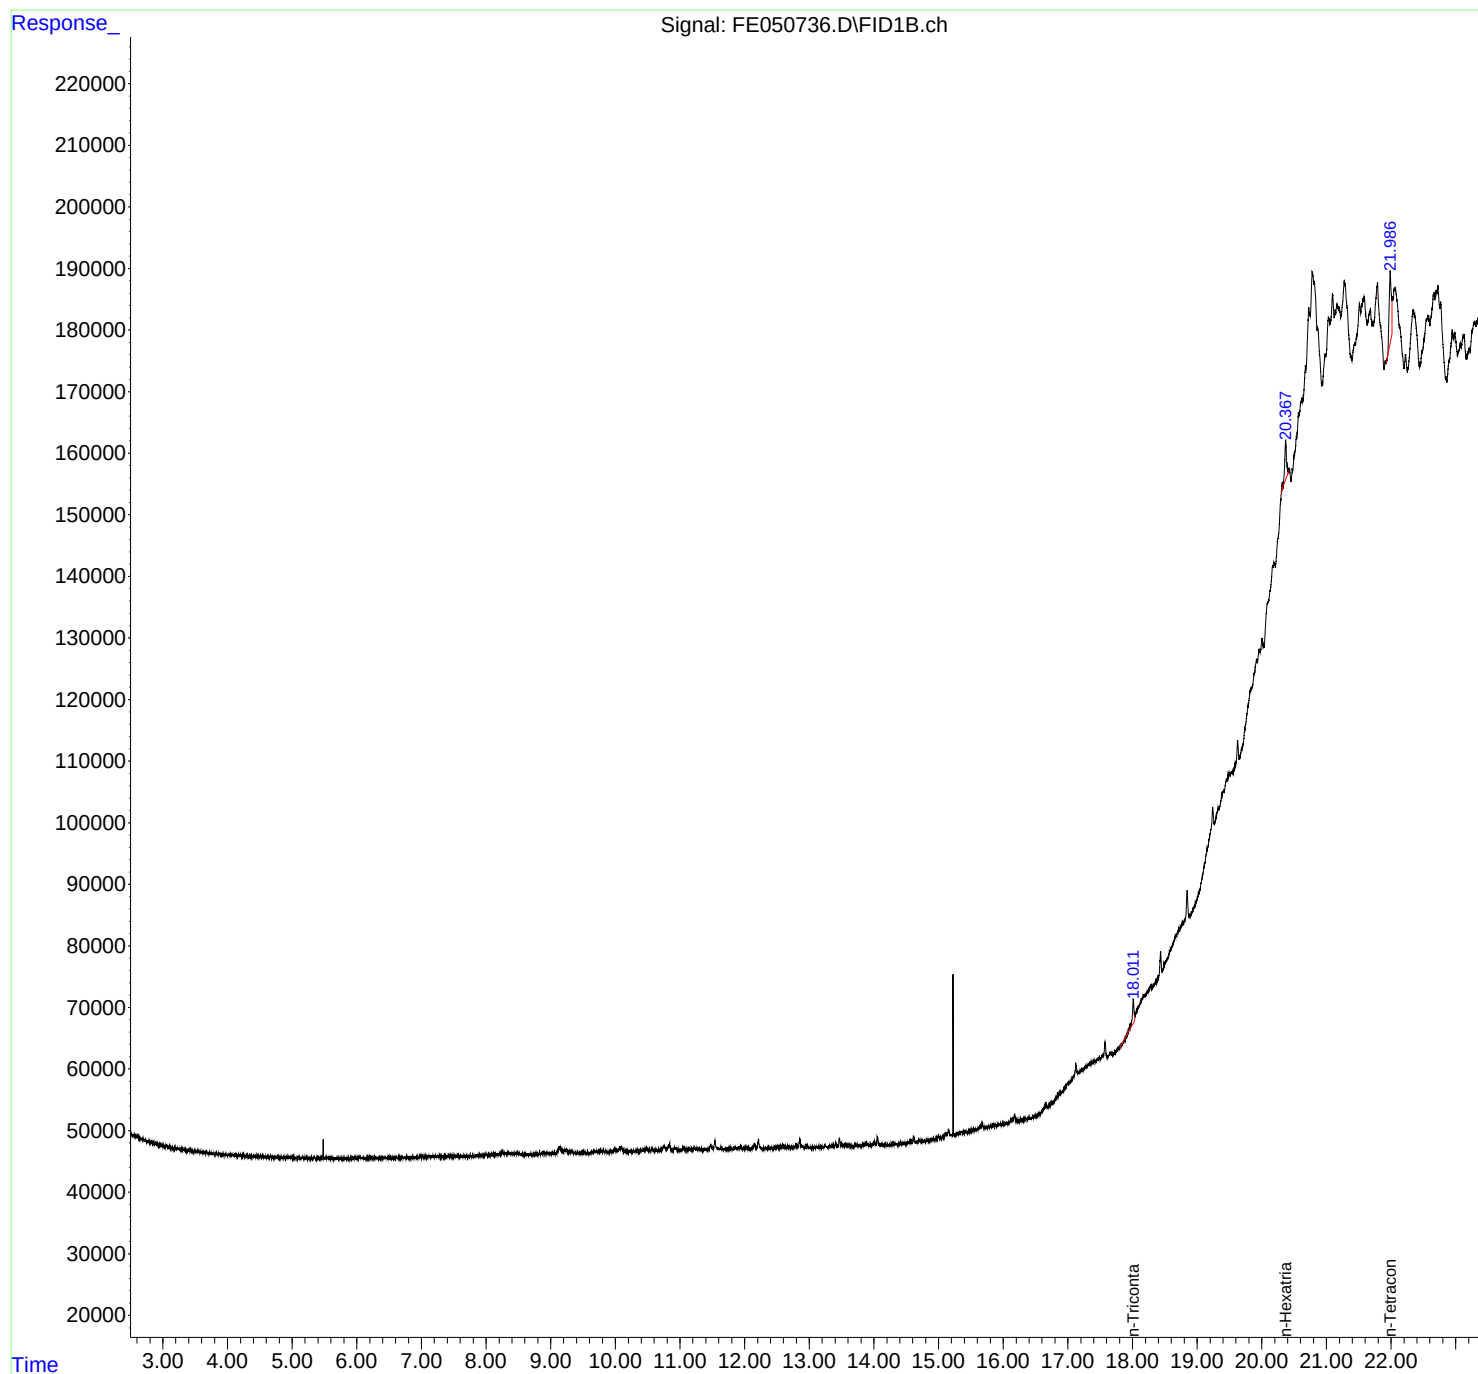


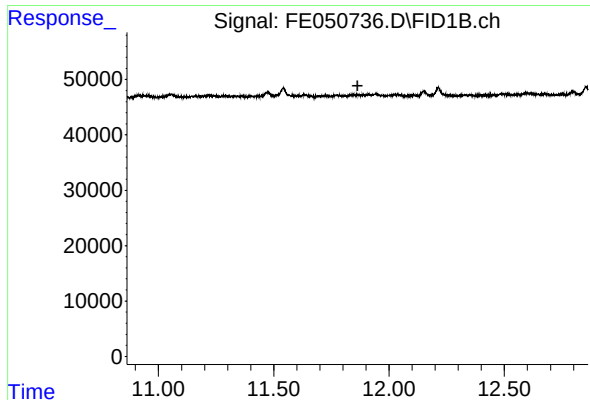

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.863 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

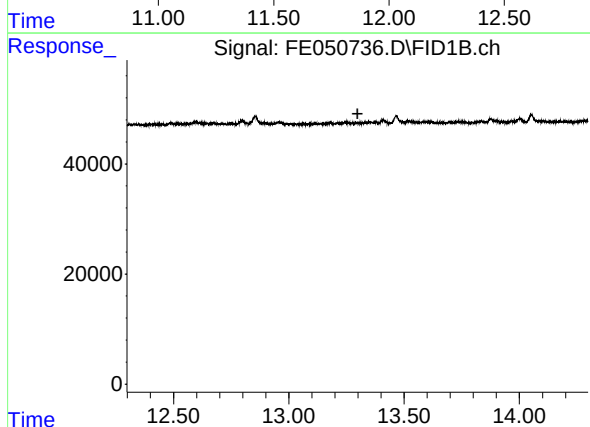


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

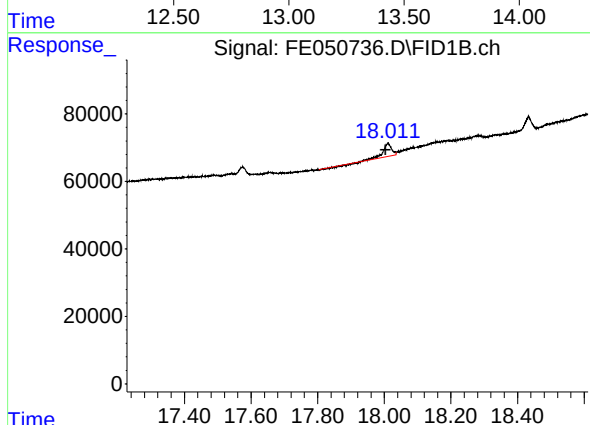


#17 n-Tricontane (C30)

R.T.: 18.011 min
Delta R.T.: 0.007 min
Response: 61980
Conc: 0.39 ug/ml

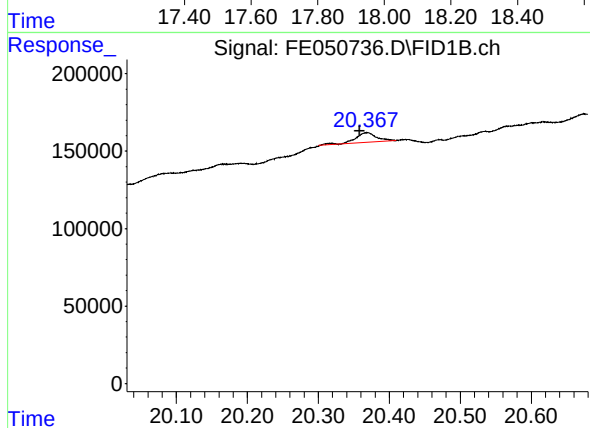

#20 n-Hexatriacontane (C36)

R.T.: 20.369 min
Delta R.T.: 0.010 min
Response: 129981
Conc: 1.02 ug/ml

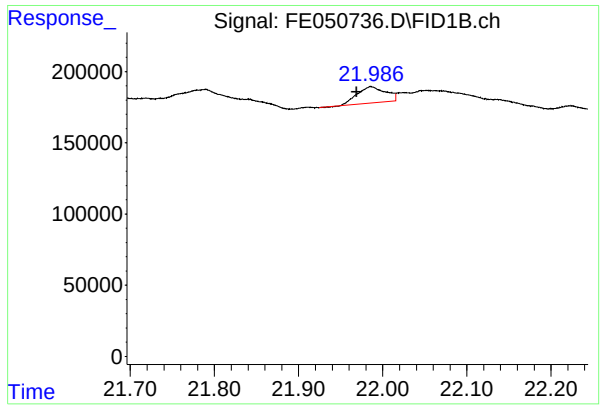

#22 n-Tetracontane (C40)

R.T.: 21.986 min
Delta R.T.: 0.017 min
Response: 273524
Conc: 2.46 ug/ml

Instrument :

FID_E

ClientSampleId :