

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102124AL\
 Data File : FE050749.D
 Signal(s) : FID1B.ch
 Acq On : 21 Oct 2024 19:08
 Operator : YP\AJ
 Sample : P4458-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 22 04:48:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 100824.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 07 16:32:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.866	5425937	34.416 ug/ml
Spiked Amount 50.000		Recovery =	68.83%
12) S 1-chlorooctadecane (S...	13.301	4350895	36.781 ug/ml
Spiked Amount 50.000		Recovery =	73.56%
Target Compounds			
14) T n-Tetracosane (C24)	15.155	221902	1.571 ug/ml
16) T n-Octacosane (C28)	17.119	111890	0.765 ug/ml
17) T n-Tricontane (C30)	18.005	368672	2.319 ug/ml
18) T n-Dotriacontane (C32)	18.838	223612	1.379 ug/ml
19) T n-Tetratriacontane (C34)	19.622	152375	1.037 ug/ml
20) T n-Hexatriacontane (C36)	20.365	102814	0.811 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102124AL\
Data File : FE050749.D
Signal(s) : FID1B.ch
Acq On : 21 Oct 2024 19:08
Operator : YP\AJ
Sample : P4458-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 22 04:48:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 100824.M
Quant Title : GC Extractables
QLast Update : Mon Oct 07 16:32:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

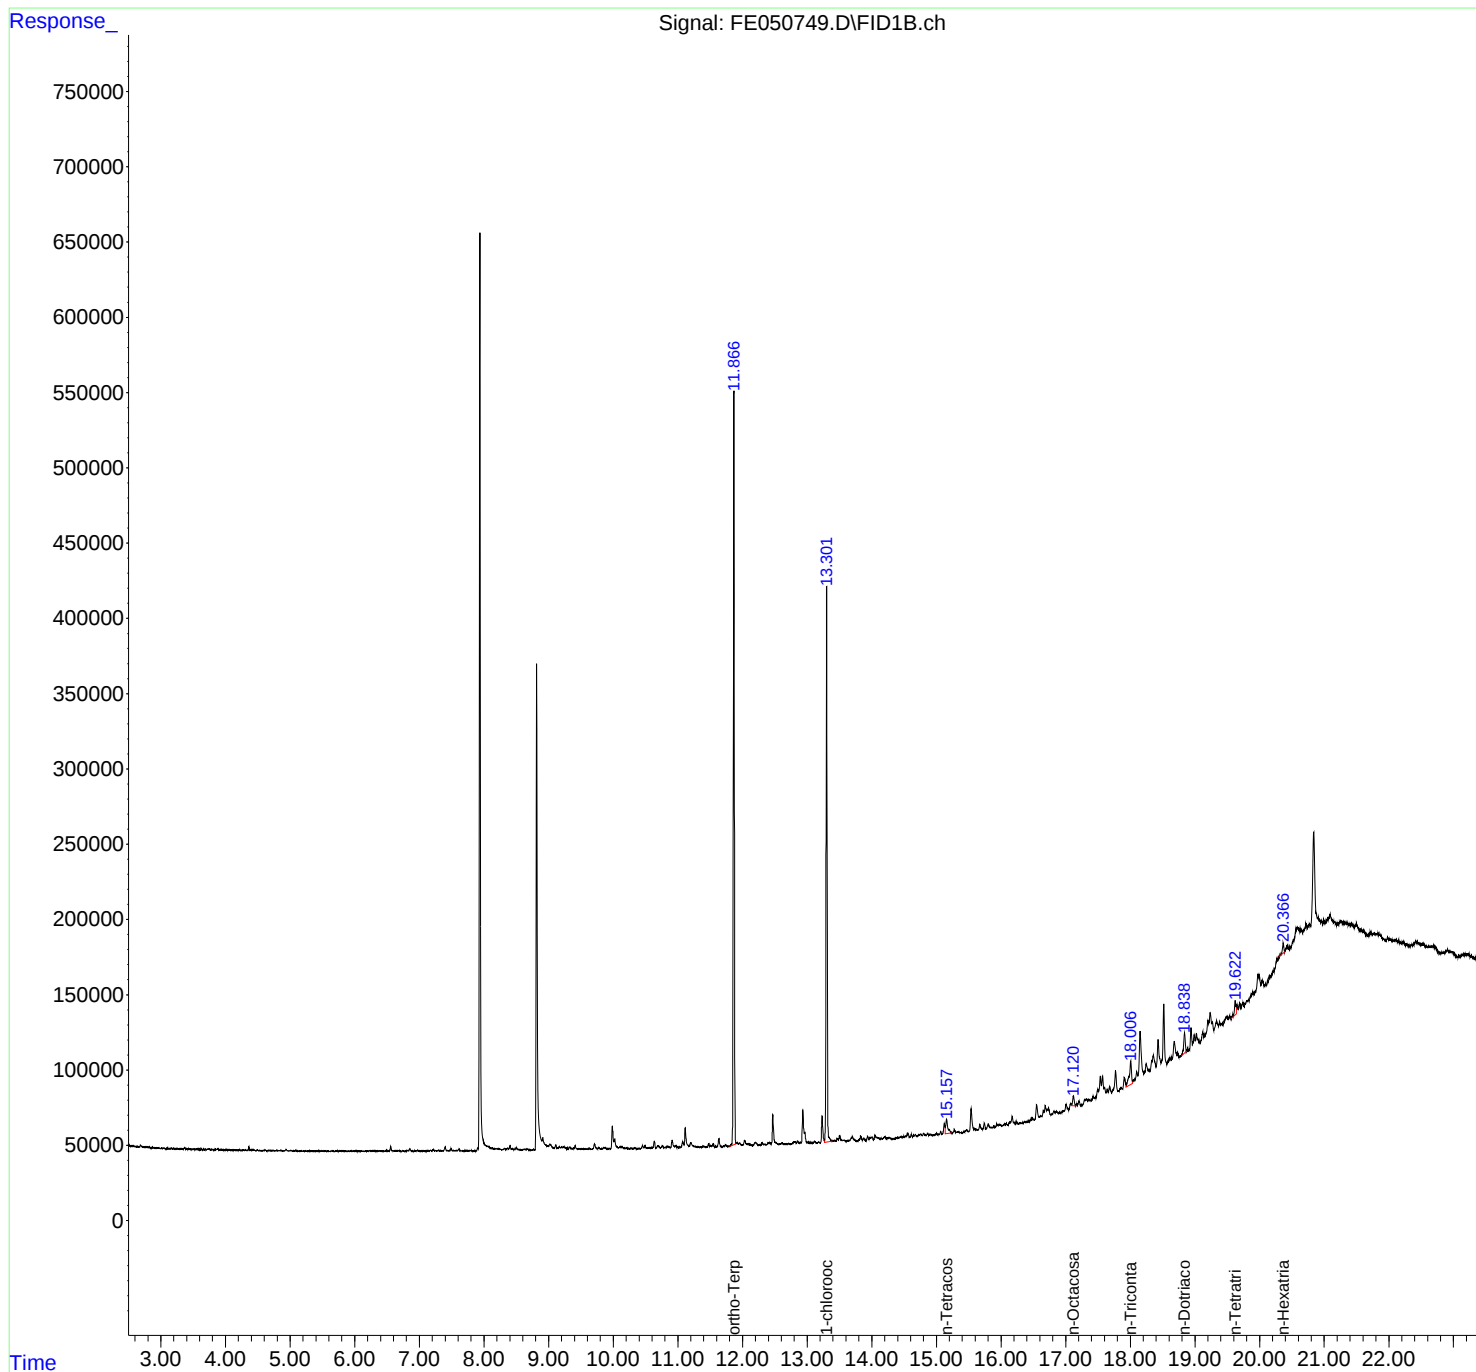


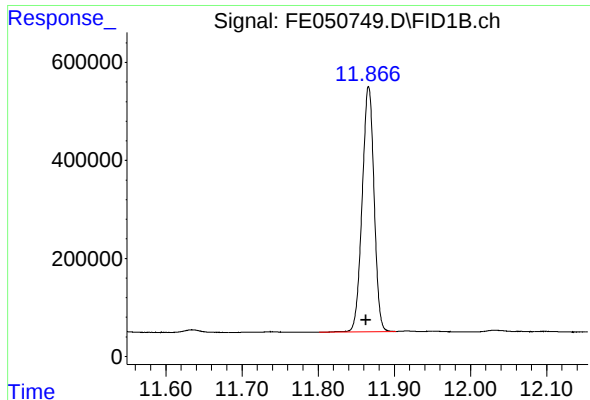

#9 ortho-Terphenyl (SURR)


R.T.: 11.866 min
Delta R.T.: 0.003 min
Response: 5425937
Conc: 34.42 ug/ml

Instrument :
FID_E
ClientSampleId :

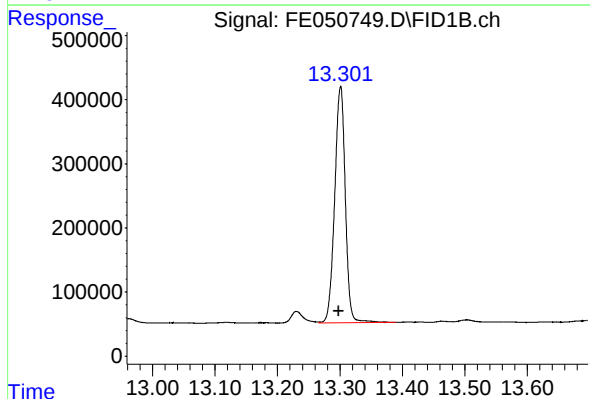


#12 1-chlorooctadecane (SURR)

R.T.: 13.301 min
Delta R.T.: 0.003 min
Response: 4350895
Conc: 36.78 ug/ml

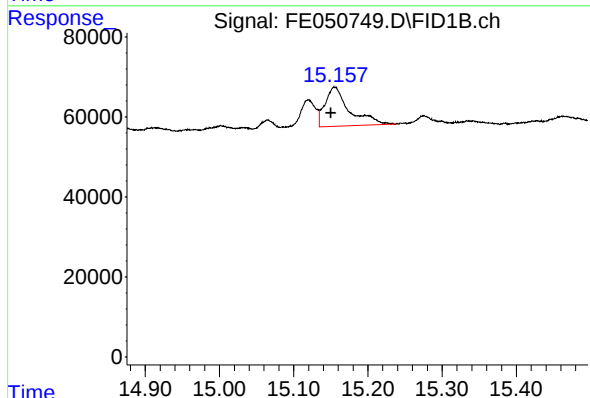


#14 n-Tetracosane (C24)

R.T.: 15.155 min
Delta R.T.: 0.005 min
Response: 221902
Conc: 1.57 ug/ml

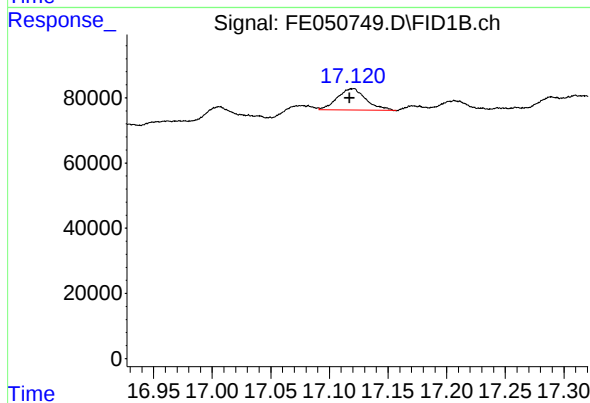

#16 n-Octacosane (C28)


R.T.: 17.119 min
Delta R.T.: 0.002 min
Response: 111890
Conc: 0.76 ug/ml

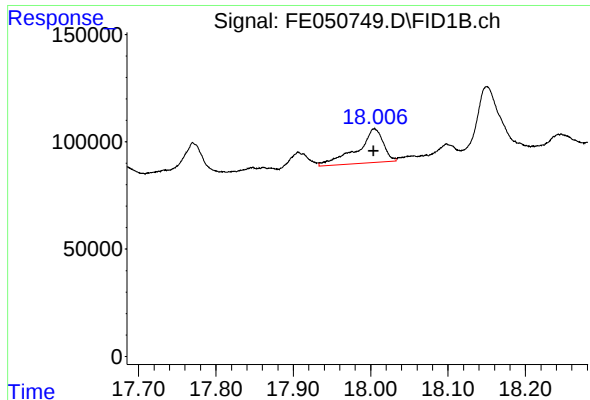

#17 n-Tricontane (C30)


R.T.: 18.005 min
Delta R.T.: 0.000 min
Response: 368672
Conc: 2.32 ug/ml

Instrument :
FID_E
ClientSampleId :

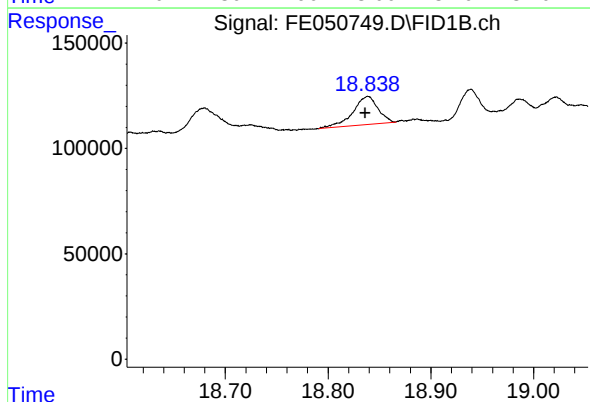


#18 n-Dotriacontane (C32)

R.T.: 18.838 min
Delta R.T.: 0.002 min
Response: 223612
Conc: 1.38 ug/ml

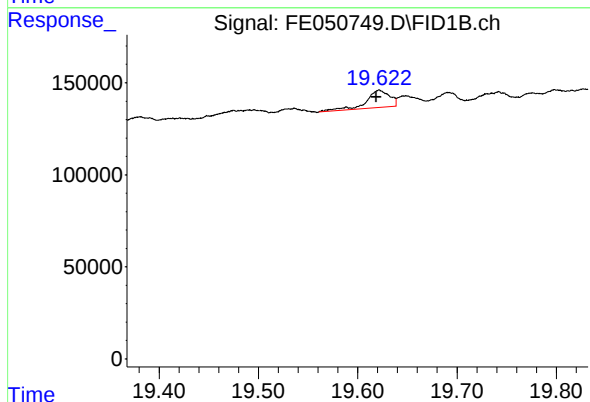

#19 n-Tetratriacontane (C34)

R.T.: 19.622 min
Delta R.T.: 0.003 min
Response: 152375
Conc: 1.04 ug/ml

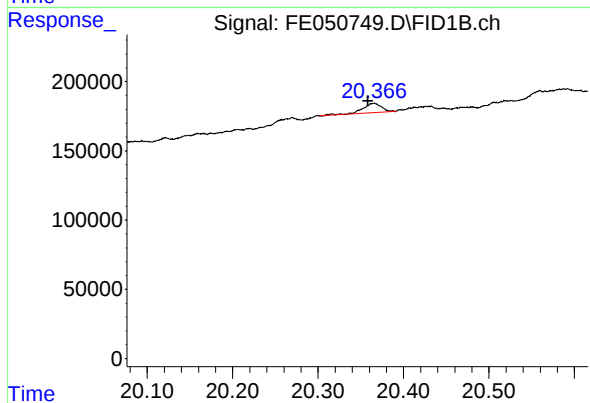

#20 n-Hexatriacontane (C36)

R.T.: 20.365 min
Delta R.T.: 0.007 min
Response: 102814
Conc: 0.81 ug/ml