

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE102325AL\  
Data File : FE056458.D  
Signal(s) : FID1B.ch  
Acq On : 23 Oct 2025 10:28  
Operator : YP\AJ  
Sample : Q3404-07DL 1000X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
MOO-25-0292-EPH-2DL

Integration File: autoint1.e  
Quant Time: Oct 23 13:28:17 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 101725.M  
Quant Title : GC Extractables  
QLast Update : Fri Oct 17 08:31:49 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| Target Compounds            |      |          |            |
| -----                       |      |          |            |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE102325AL\  
Data File : FE056458.D  
Signal(s) : FID1B.ch  
Acq On : 23 Oct 2025 10:28  
Operator : YP\AJ  
Sample : Q3404-07DL 1000X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
MOO-25-0292-EPH-2DL

Integration File: autoint1.e  
Quant Time: Oct 23 13:28:17 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 101725.M  
Quant Title : GC Extractables  
QLast Update : Fri Oct 17 08:31:49 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

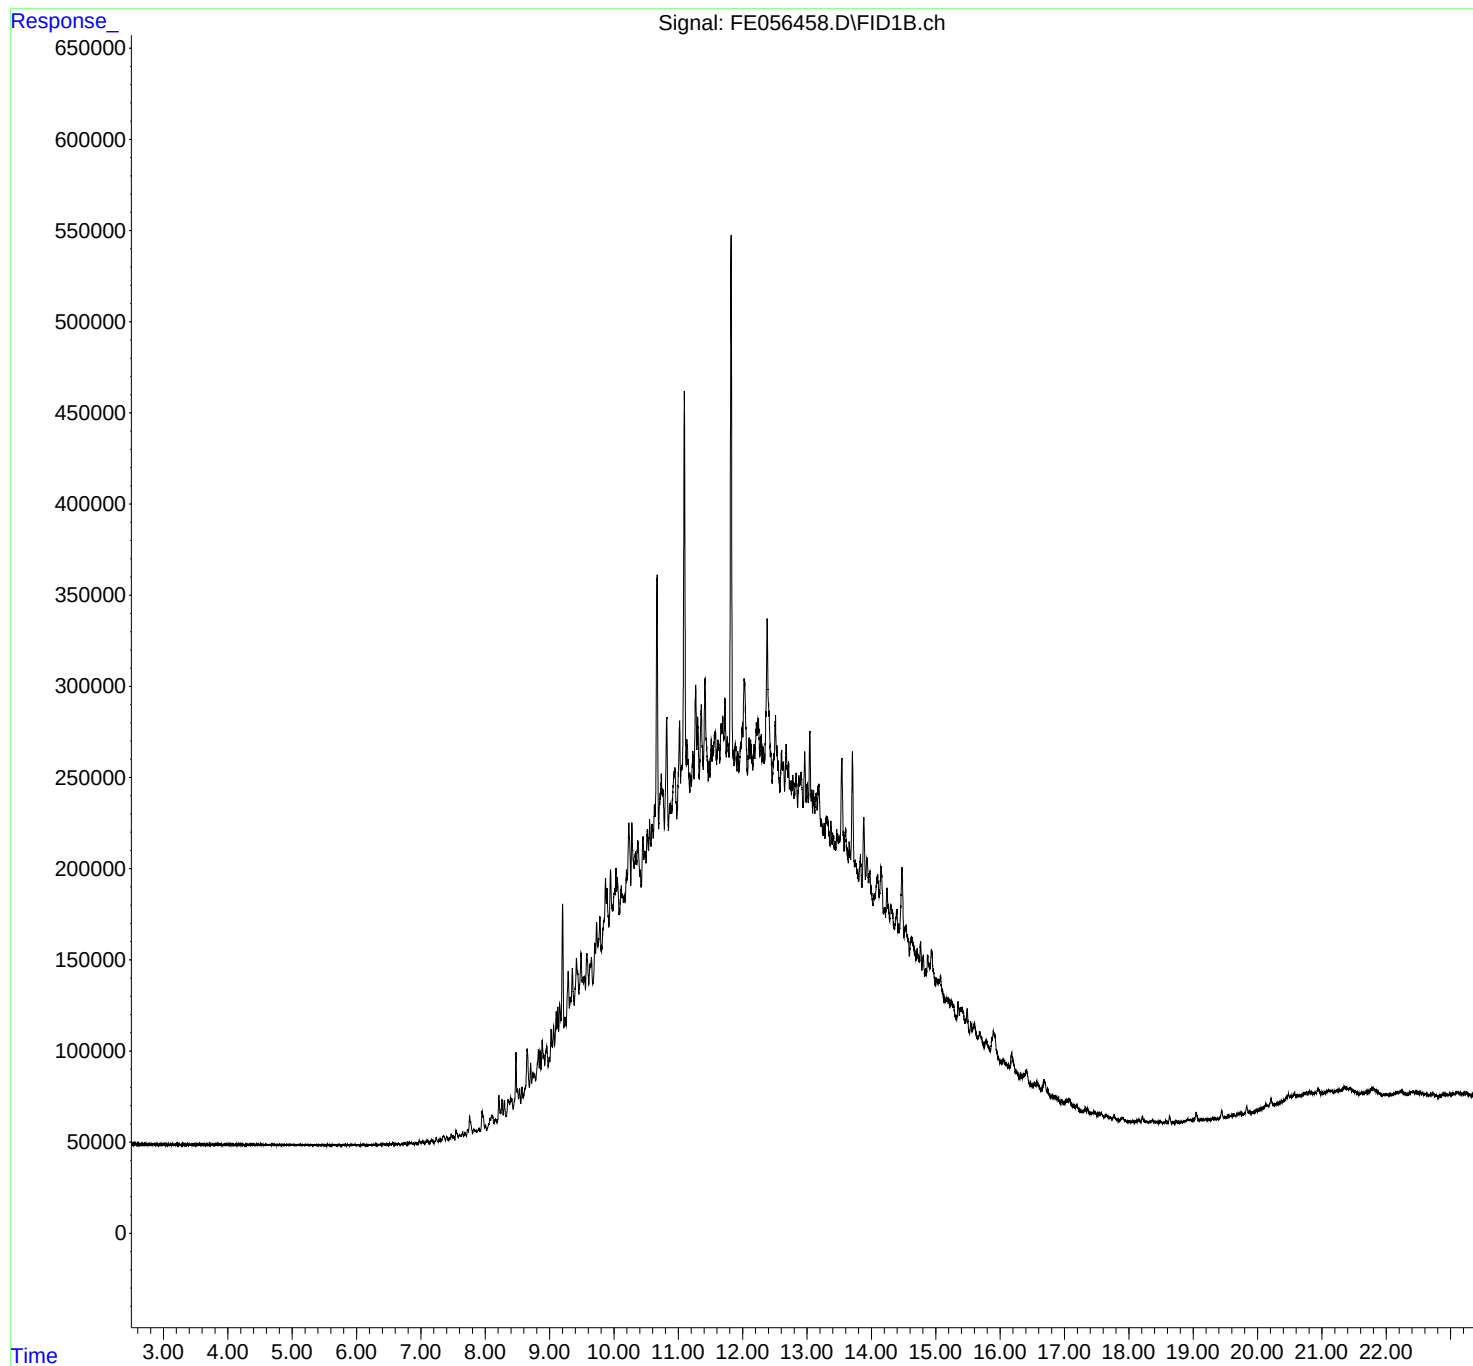


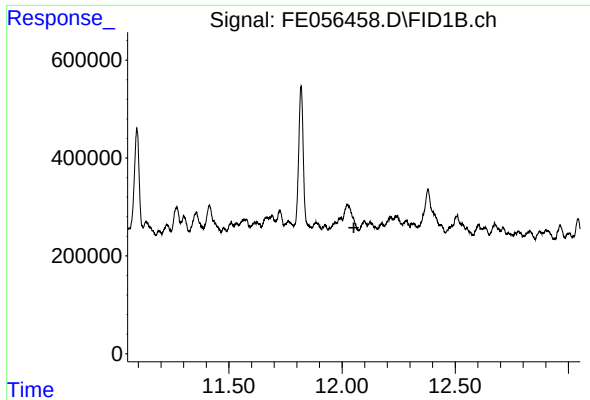

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T. : 12.052 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
MOO-25-0292-EPH-2DL

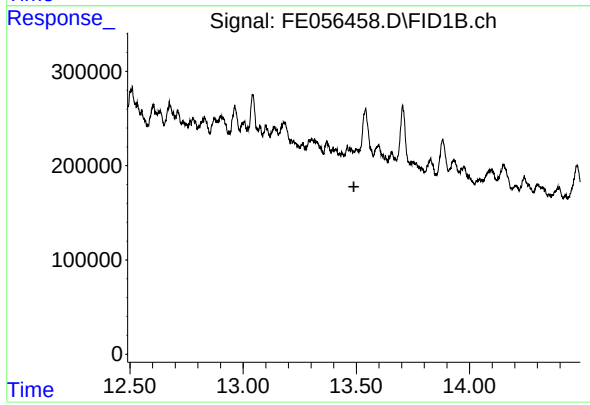

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T. : 13.489 min  
Response: 0  
Conc: N.D.