

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE102524AL\  
 Data File : FE050842.D  
 Signal(s) : FID1B.ch  
 Acq On : 25 Oct 2024 17:46  
 Operator : YP\AJ  
 Sample : P4547-01  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 BP-F-21

Integration File: autoint1.e  
 Quant Time: Oct 26 01:36:32 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 100824.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Oct 07 16:32:18 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.860 | 7608561    | 48.261 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 96.52%       |
| 12) S 1-chlorooctadecane (S... | 13.294 | 6110438    | 51.655 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 103.31%      |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE102524AL\  
Data File : FE050842.D  
Signal(s) : FID1B.ch  
Acq On : 25 Oct 2024 17:46  
Operator : YP\AJ  
Sample : P4547-01  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
BP-F-21

Integration File: autoint1.e  
Quant Time: Oct 26 01:36:32 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 100824.M  
Quant Title : GC Extractables  
QLast Update : Mon Oct 07 16:32:18 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

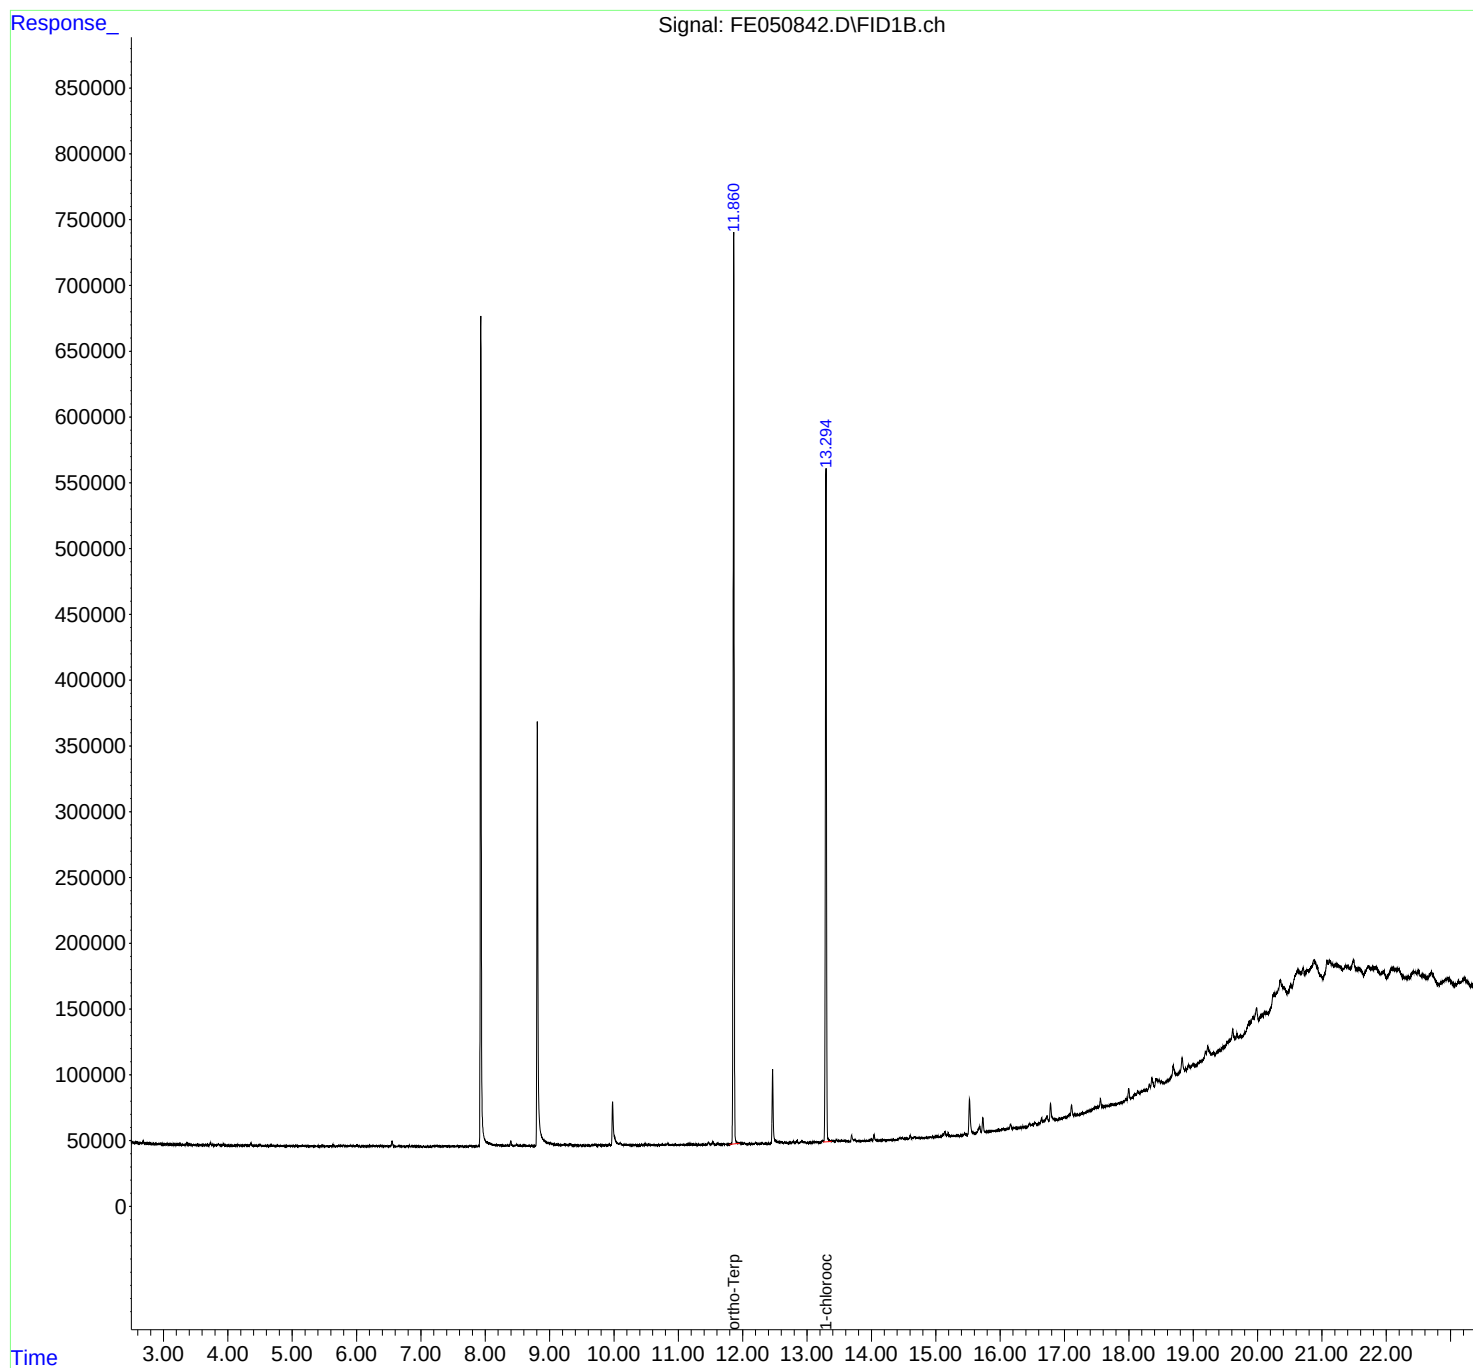


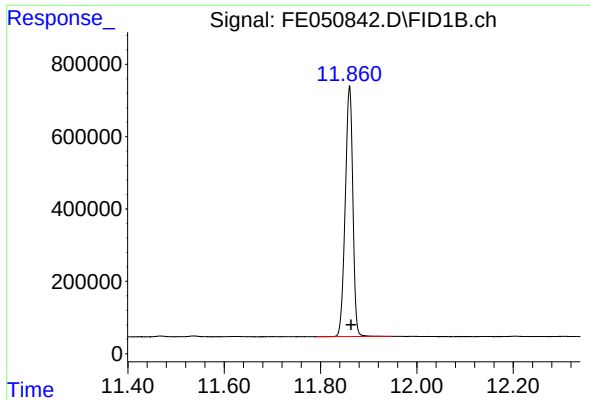

#9 ortho-Terphenyl (SURR)

R.T.: 11.860 min  
Delta R.T.: -0.003 min  
Response: 7608561  
Conc: 48.26 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
BP-F-21

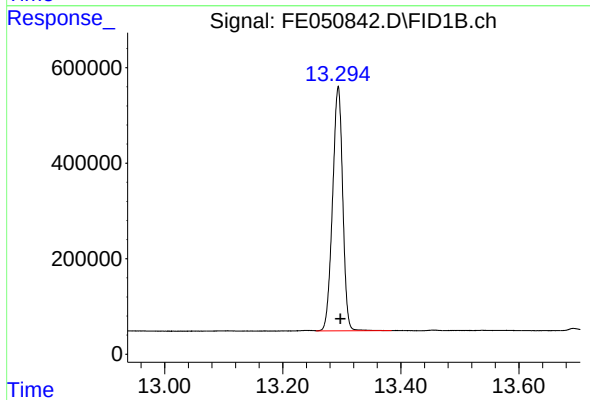

#12 1-chlorooctadecane (SURR)

R.T.: 13.294 min  
Delta R.T.: -0.004 min  
Response: 6110438  
Conc: 51.65 ug/ml