

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE102618\  
Data File : FE028966.D  
Signal(s) : FID1B.CH  
Acq On : 26 Oct 2018 13:00  
Operator : DD\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Oct 27 04:56:07 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE102318.M  
Quant Title :  
QLast Update : Wed Oct 24 08:22:18 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

| Compound                    |                 | R.T.   | Response | Conc Units  |
|-----------------------------|-----------------|--------|----------|-------------|
| -----                       |                 |        |          |             |
| System Monitoring Compounds |                 |        |          |             |
| Target Compounds            |                 |        |          |             |
| 10)                         | N-TETRACOSANE   | 15.105 | 155017   | 1.085 ug/ml |
| 11)                         | N-OCTACOSANE    | 17.090 | 72364    | 0.532 ug/ml |
| 12)                         | N-DOTRIACONTANE | 18.831 | 274669   | 2.305 ug/ml |
| -----                       |                 |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE102618\  
Data File : FE028966.D  
Signal(s) : FID1B.CH  
Acq On : 26 Oct 2018 13:00  
Operator : DD\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Oct 27 04:56:07 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\C44-FE102318.M  
Quant Title :  
QLast Update : Wed Oct 24 08:22:18 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 uL  
Signal Phase : Rxi-1ms  
Signal Info : 20m x 0.18mm x 0.18um

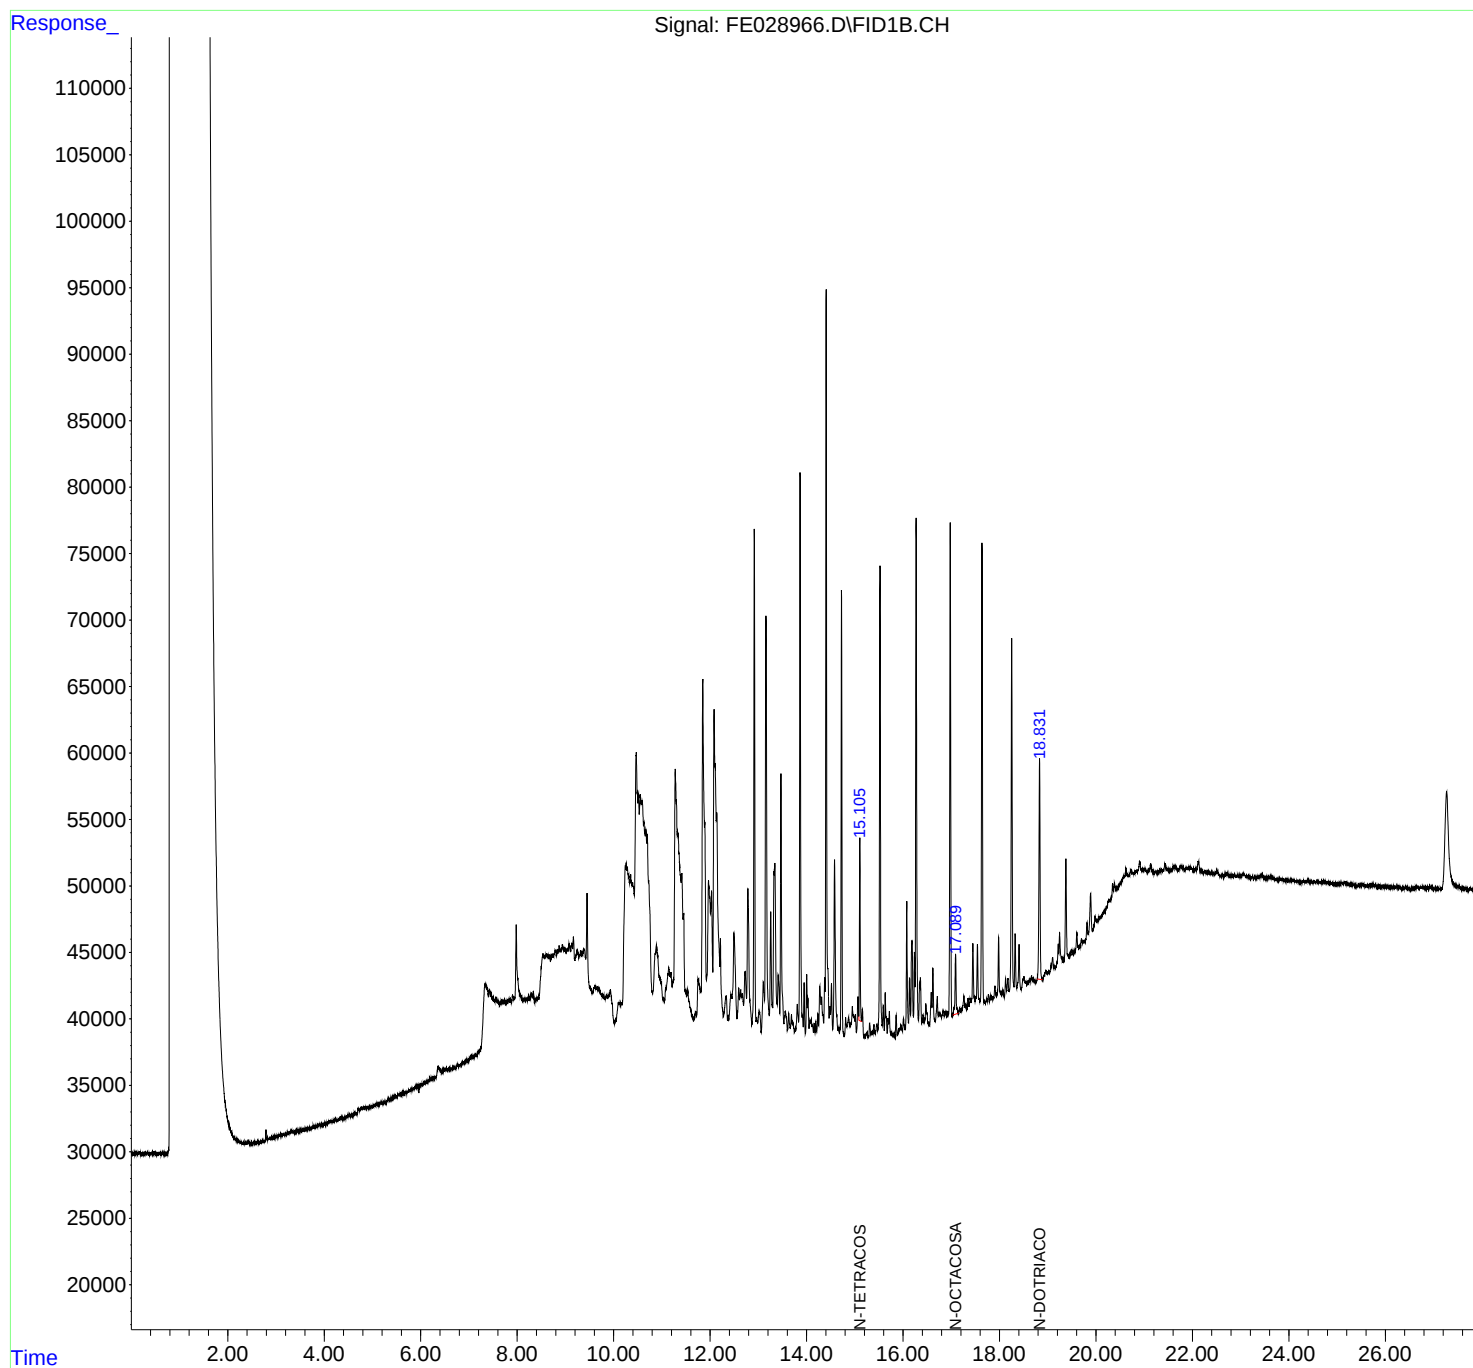

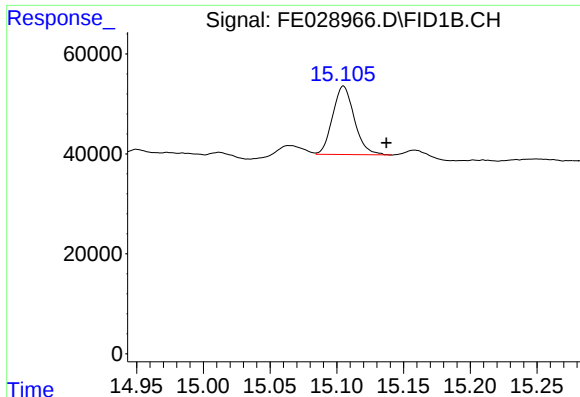


#10 N-TETRACOSANE

R.T.: 15.105 min  
Delta R.T.: -0.032 min  
Response: 155017  
Conc: 1.08 ug/ml

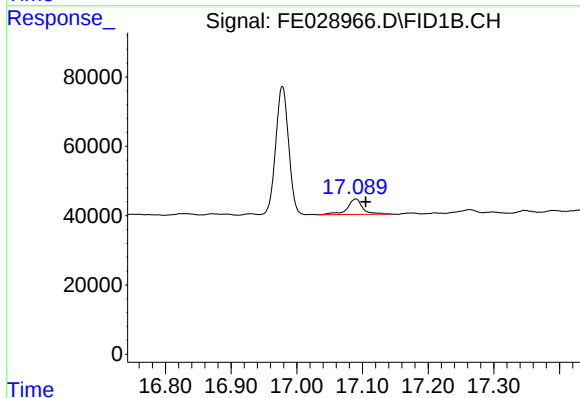


#11 N-OCTACOSANE

R.T.: 17.090 min  
Delta R.T.: -0.015 min  
Response: 72364  
Conc: 0.53 ug/ml

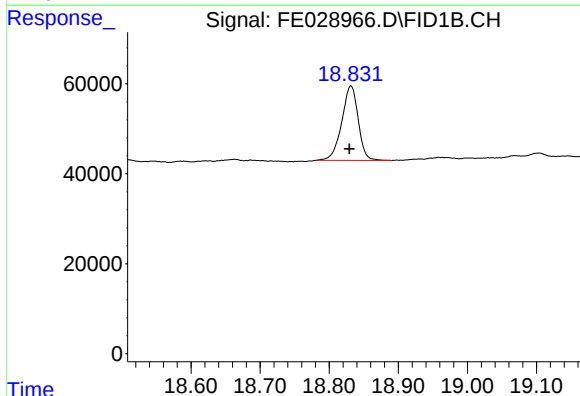

#12 N-DOTRIACONTANE

R.T.: 18.831 min  
Delta R.T.: 0.002 min  
Response: 274669  
Conc: 2.30 ug/ml

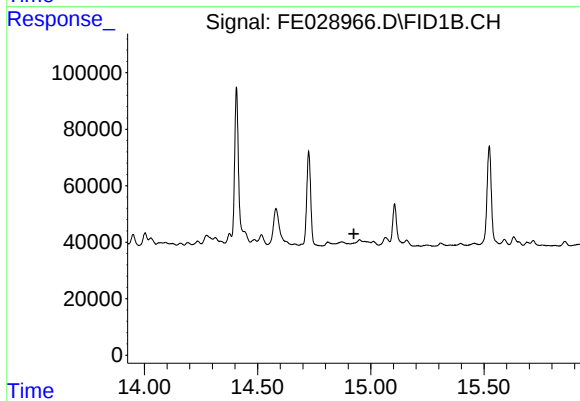

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.925 min  
Response: 0  
Conc: N.D.