

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102622\
Data File : FE038317.D
Signal(s) : FID1B.ch
Acq On : 26 Oct 2022 10:56
Operator : YP\AJ
Sample : N5235-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
LSP-GW-03-DUP

Integration File: autoint1.e
Quant Time: Oct 27 06:34:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102522.M
Quant Title :
QLast Update : Wed Oct 26 13:27:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	15.070	2521925	19.518 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102622\
Data File : FE038317.D
Signal(s) : FID1B.ch
Acq On : 26 Oct 2022 10:56
Operator : YP\AJ
Sample : N5235-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
LSP-GW-03-DUP

Integration File: autoint1.e
Quant Time: Oct 27 06:34:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102522.M
Quant Title :
QLast Update : Wed Oct 26 13:27:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

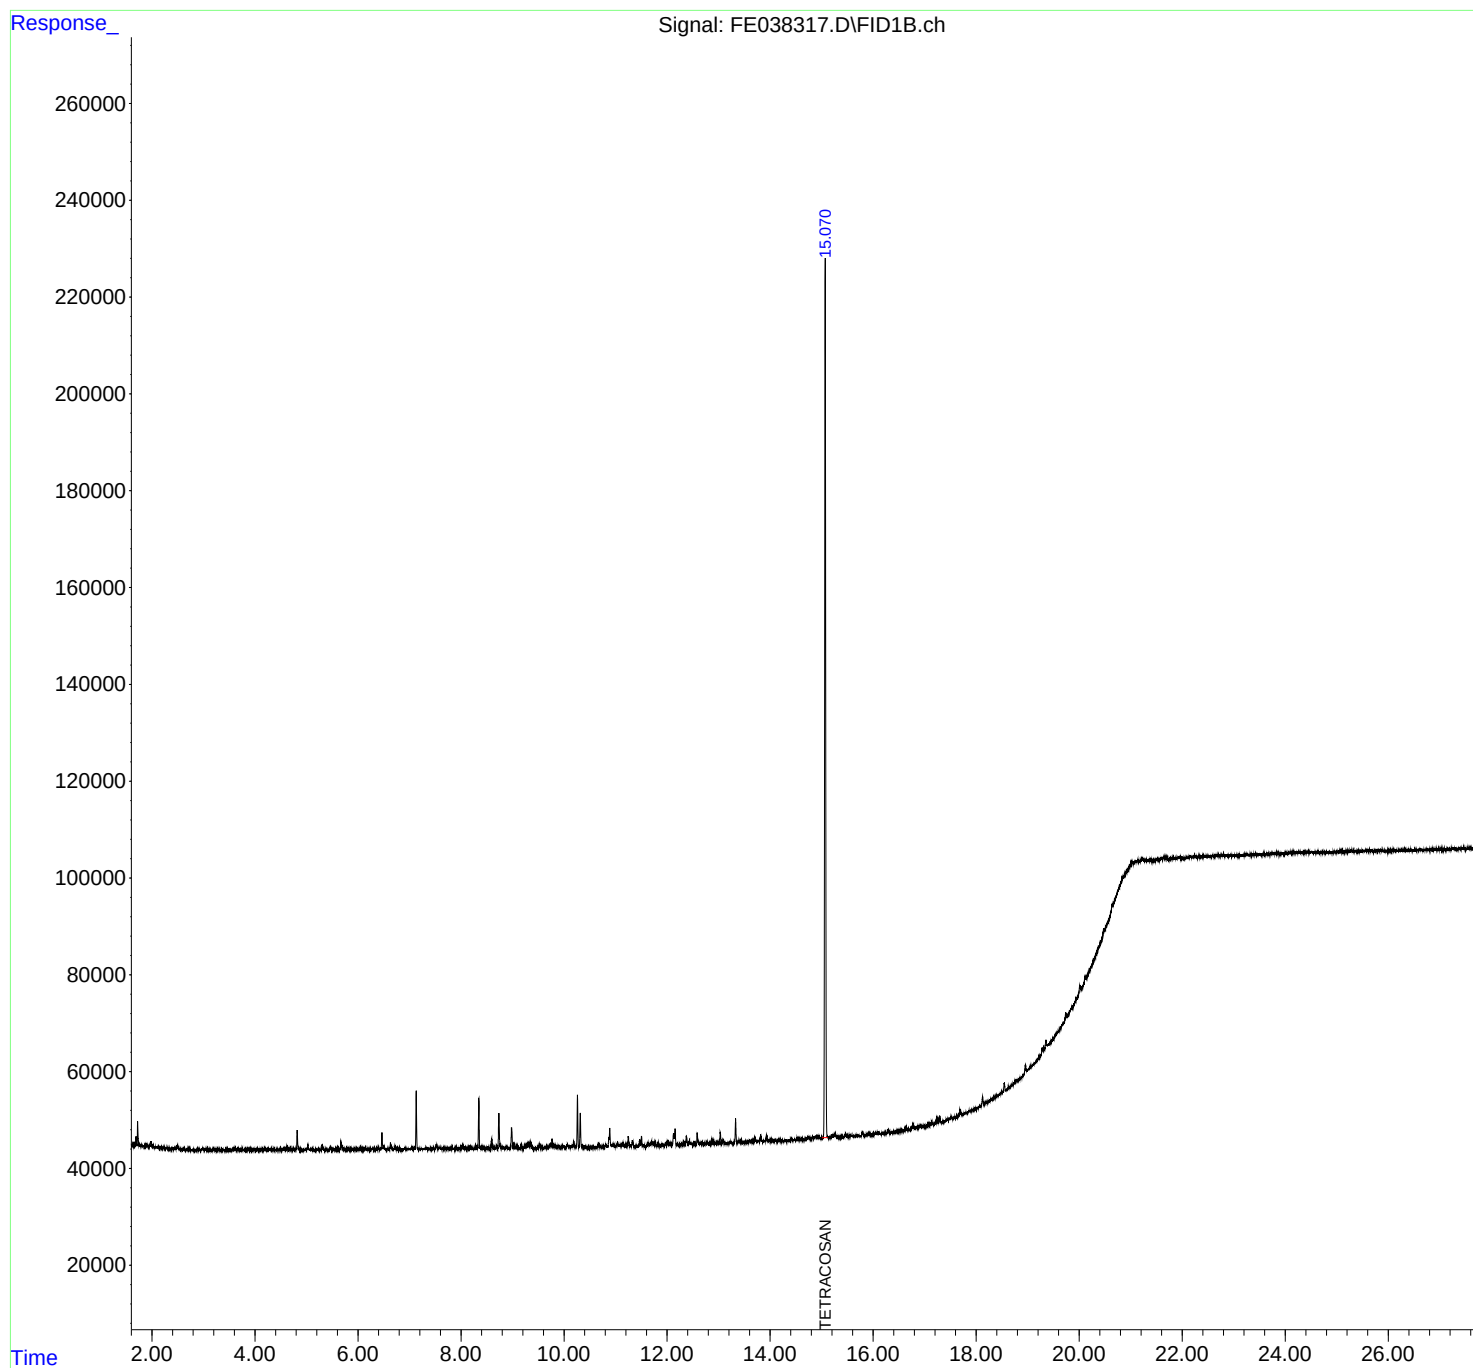

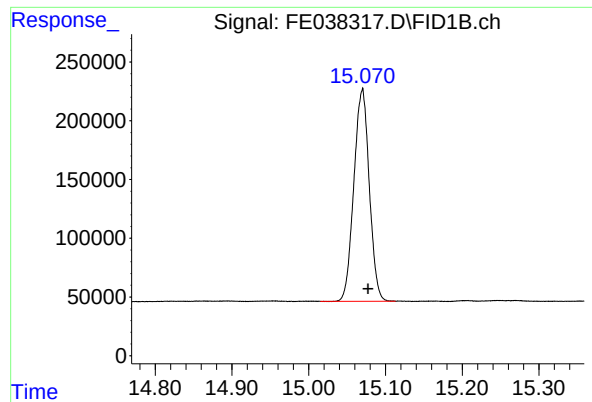

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.070 min
Delta R.T.: -0.008 min
Response: 2521925
Conc: 19.52 ug/ml

Instrument :
FID_E
ClientSampleId :
LSP-GW-03-DUP