

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102622\
Data File : FE038322.D
Signal(s) : FID1B.ch
Acq On : 26 Oct 2022 13:56
Operator : YP\AJ
Sample : N5236-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
LSP-GW-03

Integration File: autoint1.e
Quant Time: Oct 27 06:35:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102522.M
Quant Title :
QLast Update : Wed Oct 26 13:27:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	15.069	2204452	17.061 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102622\
Data File : FE038322.D
Signal(s) : FID1B.ch
Acq On : 26 Oct 2022 13:56
Operator : YP\AJ
Sample : N5236-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
LSP-GW-03

Integration File: autoint1.e
Quant Time: Oct 27 06:35:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102522.M
Quant Title :
QLast Update : Wed Oct 26 13:27:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

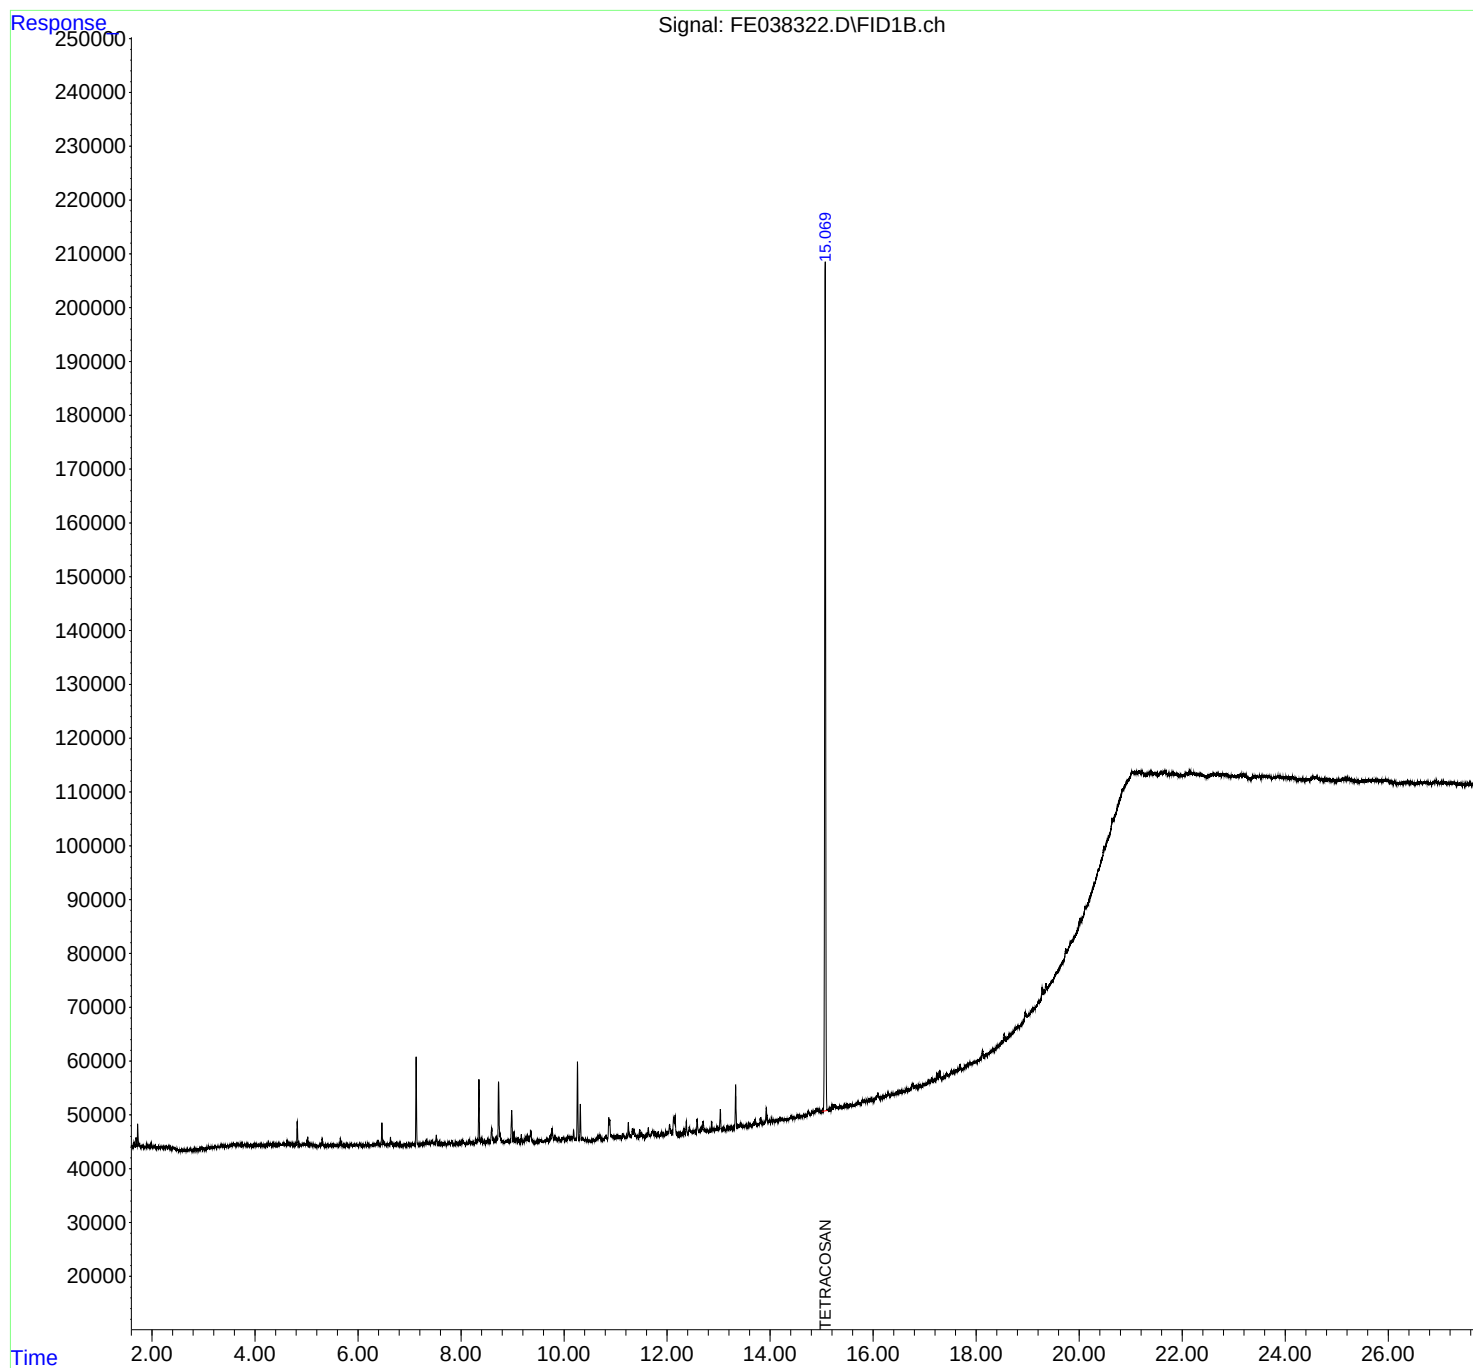

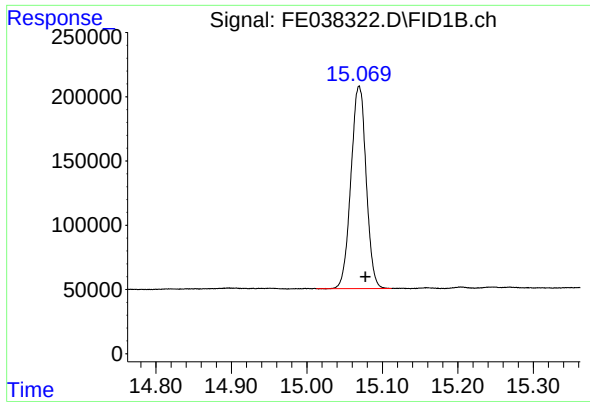

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.069 min
Delta R.T.: -0.008 min
Response: 2204452
Conc: 17.06 ug/ml

Instrument :
FID_E
ClientSampleId :
LSP-GW-03