

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102822AL\
Data File : FE038420.D
Signal(s) : FID1B.ch
Acq On : 29 Oct 2022 07:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 29 08:05:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 102522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 04:49:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.784	60340	0.409 ug/ml
20) T	n-Hexatriacontane (C36)	20.537f	49520	0.347 ug/ml
22) T	n-Tetracontane (C40)	22.142	398491	3.157 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE102822AL\
Data File : FE038420.D
Signal(s) : FID1B.ch
Acq On : 29 Oct 2022 07:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 29 08:05:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 102522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 04:49:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

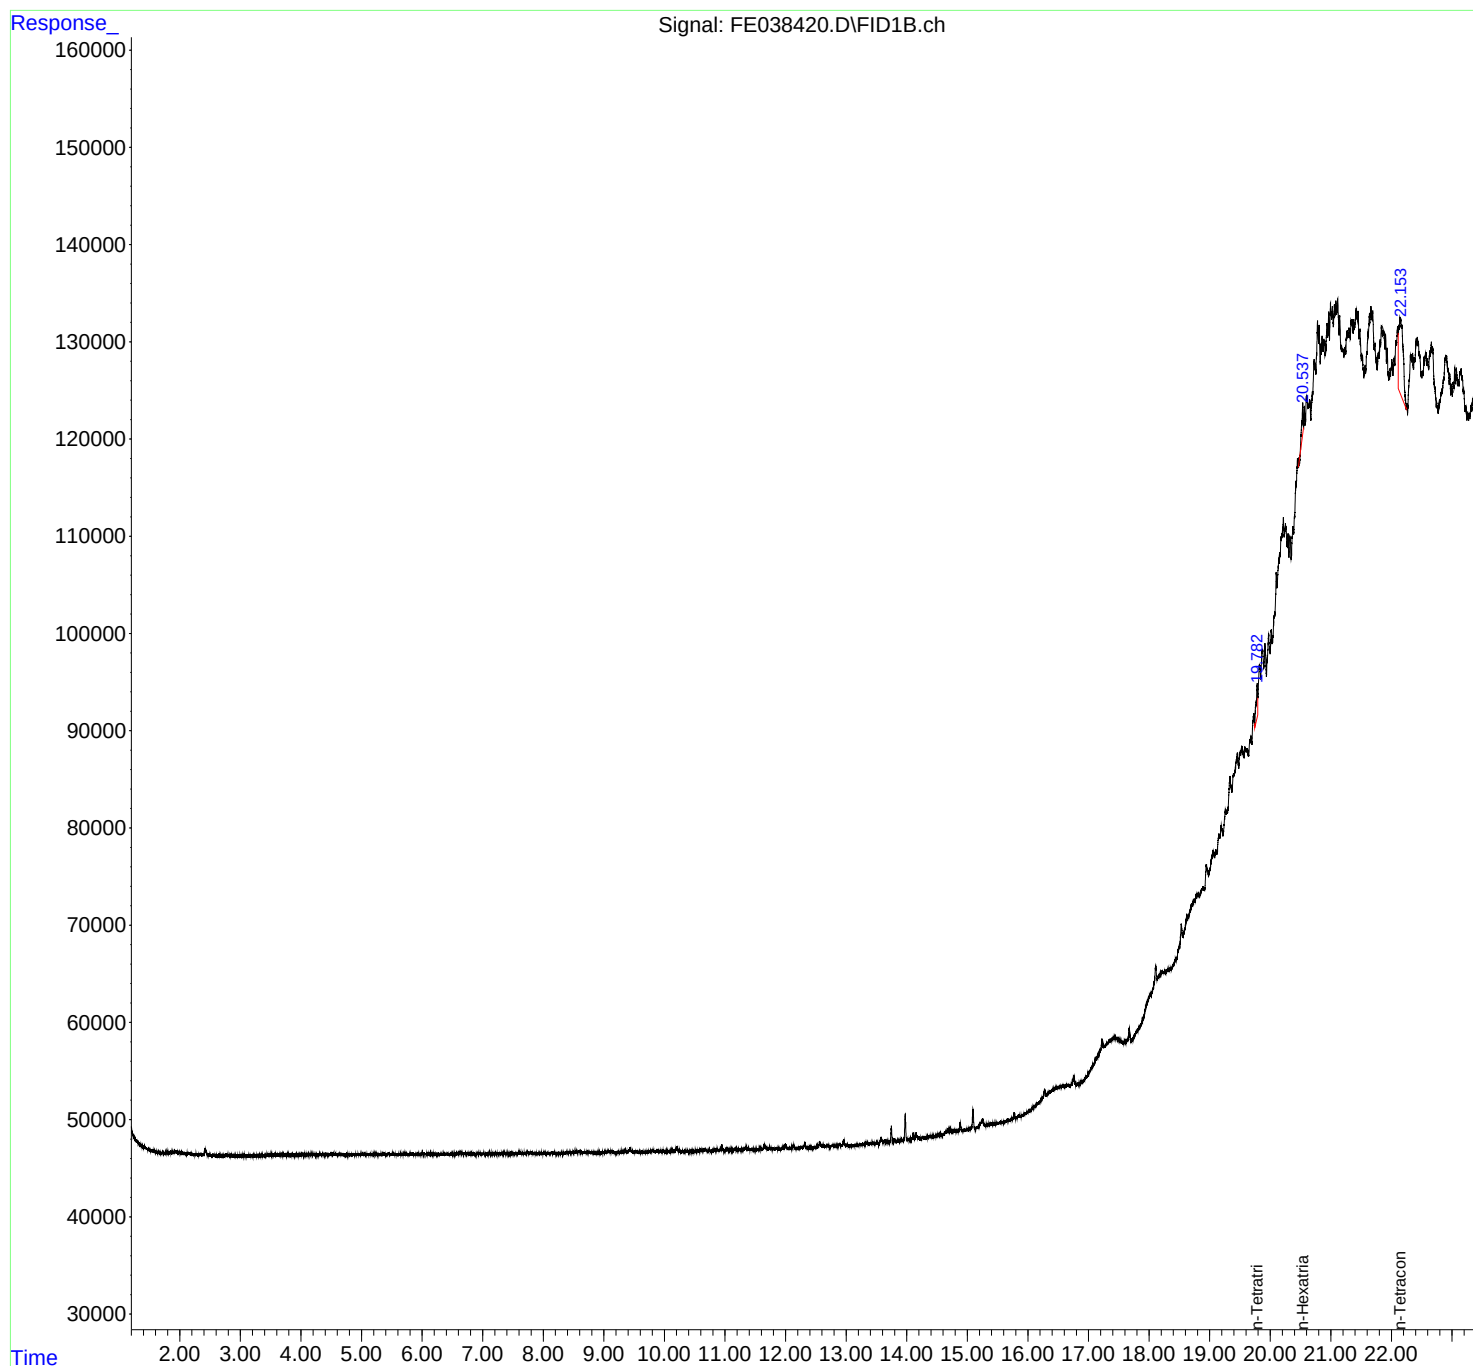


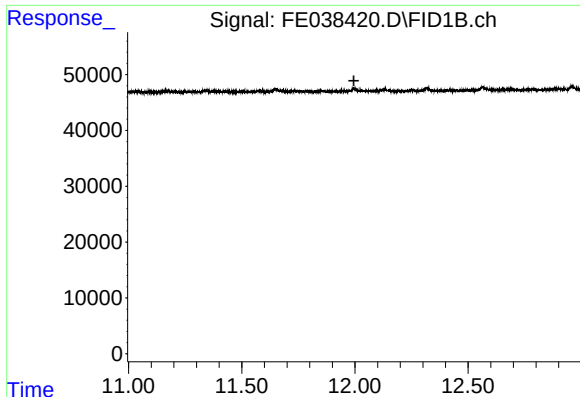

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.996 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

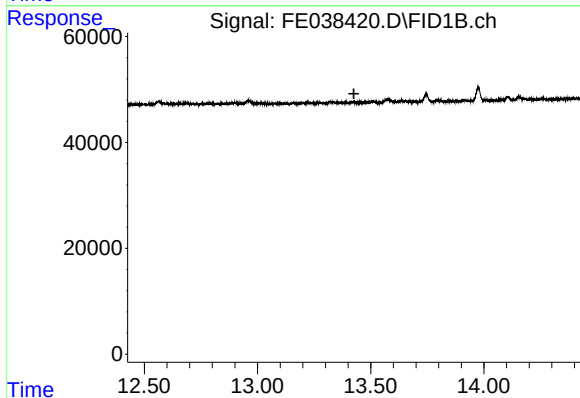


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.426 min
Response: 0
Conc: N.D.

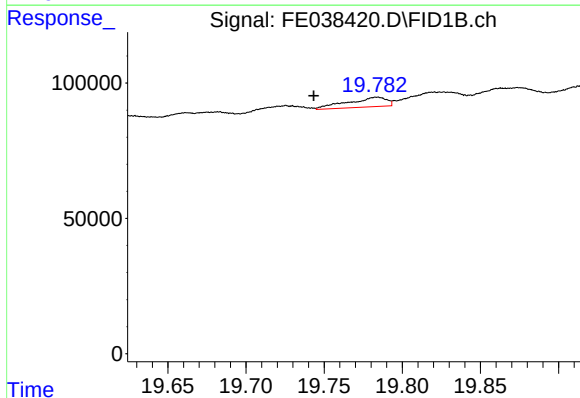


#19 n-Tetratriacontane (C34)

R.T.: 19.784 min
Delta R.T.: 0.040 min
Response: 60340
Conc: 0.41 ug/ml

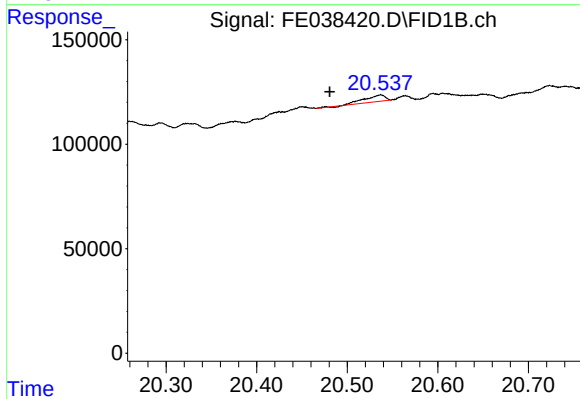

#20 n-Hexatriacontane (C36)

R.T.: 20.537 min
Delta R.T.: 0.056 min
Response: 49520
Conc: 0.35 ug/ml

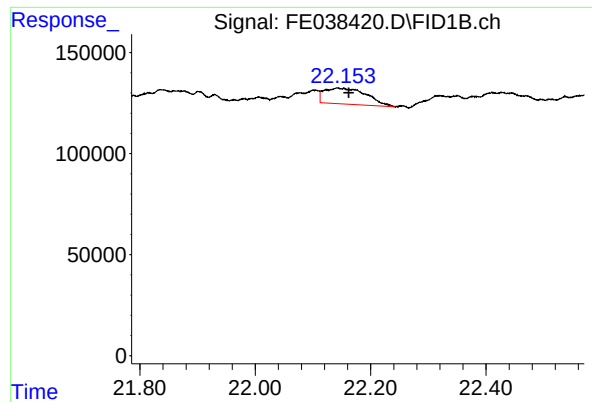

#22 n-Tetracontane (C40)

R.T.: 22.142 min
Delta R.T.: -0.020 min
Response: 398491
Conc: 3.16 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK