

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102925AR\
Data File : FG016864.D
Signal(s) : FID1A.ch
Acq On : 30 Oct 2025 01:28
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 30 06:16:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 102925.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 06:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	18.699f	12279	0.144 ug/ml
20) T	Dibenz[a,h]anthracene...	18.699	12279	0.084 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102925AR\
Data File : FG016864.D
Signal(s) : FID1A.ch
Acq On : 30 Oct 2025 01:28
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 30 06:16:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 102925.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 06:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

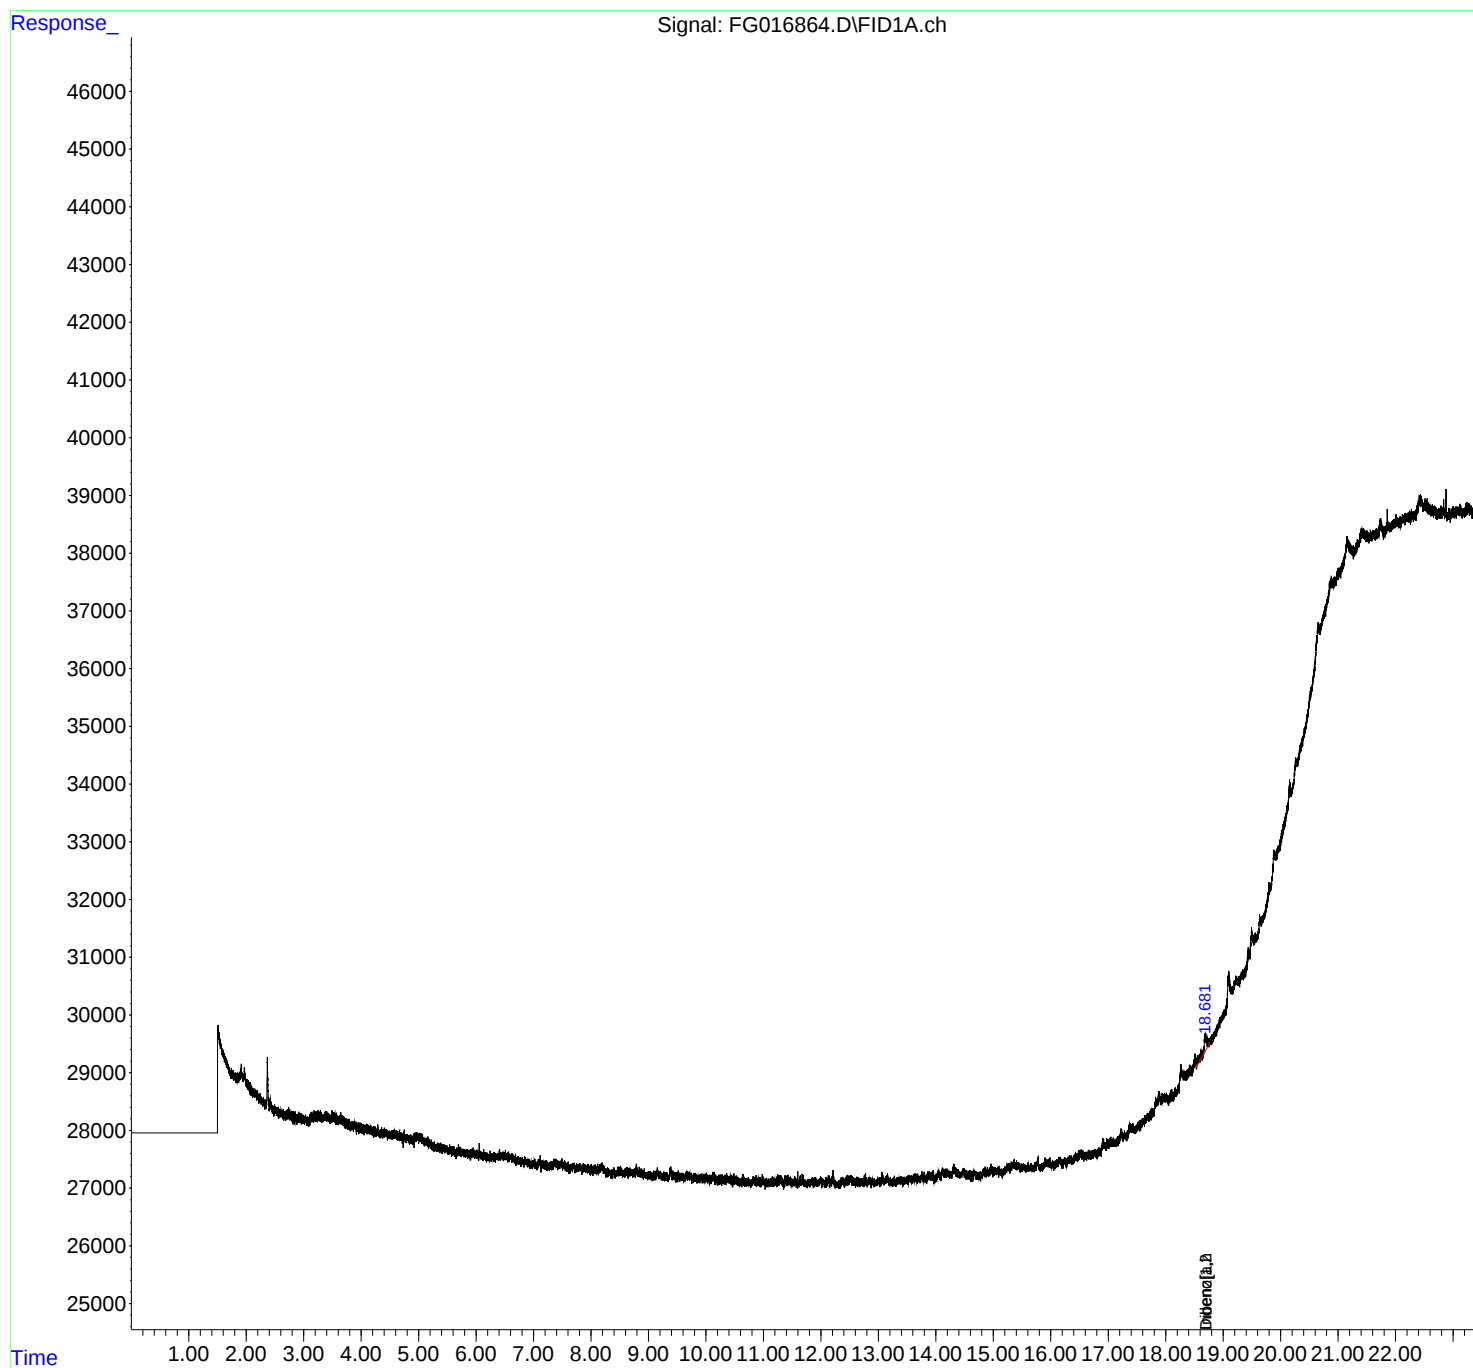


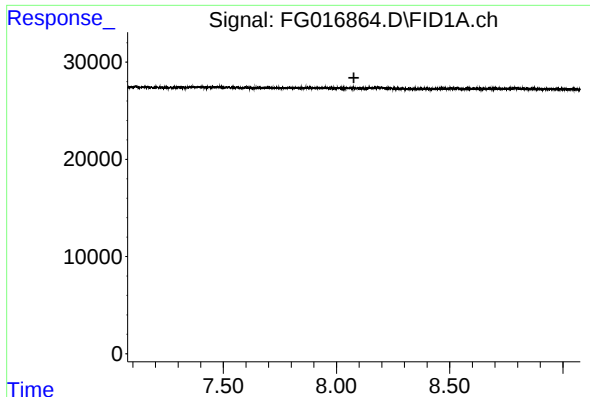

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 8.077 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

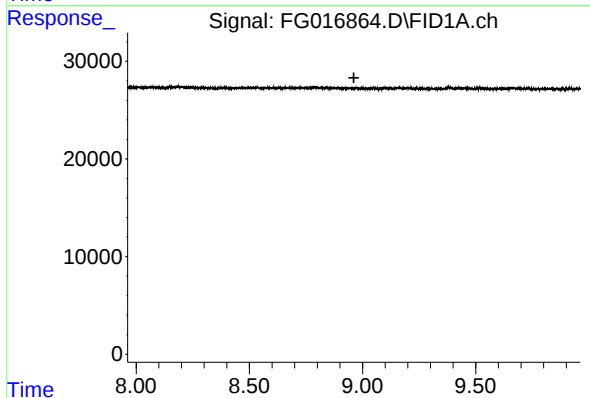


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.

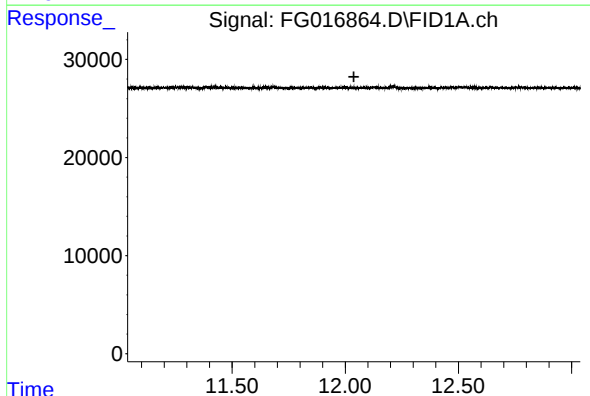


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 12.038 min
Response: 0
Conc: N.D.

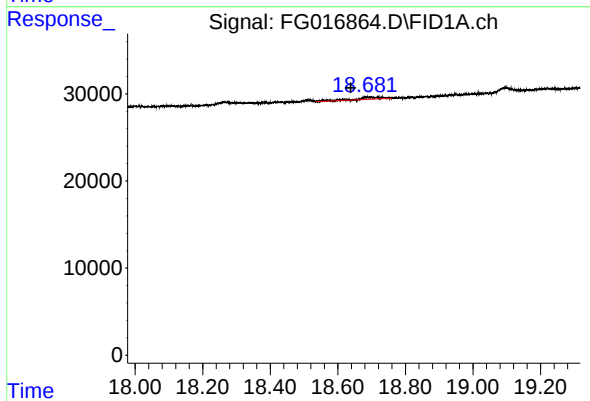

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.699 min
Delta R.T.: 0.061 min
Response: 12279
Conc: 0.14 ug/ml

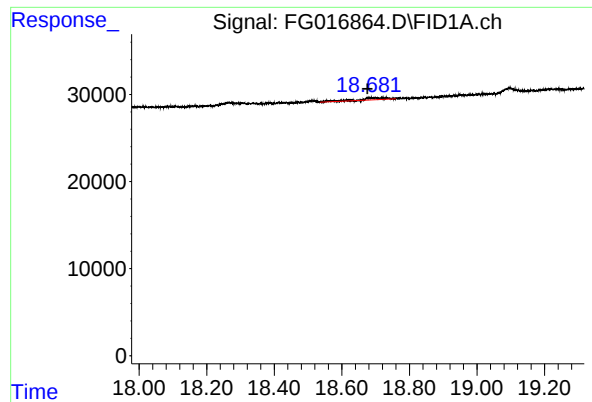

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.699 min
Delta R.T.: 0.023 min
Response: 12279
Conc: 0.08 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK