

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103018\
 Data File : FF002511.D
 Signal(s) : FID2B.ch
 Acq On : 30 Oct 2018 18:20
 Operator : AJ\SJ
 Sample : J5724-06
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 31 00:40:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	1021117	7.347 ug/ml
Target Compounds			
2) N-DECANE	4.375	85208	0.558 ug/ml
4) N-TETRADECANE	8.247f	290740	1.858 ug/ml
6) N-OCTADECANE	11.180f	131232	0.826 ug/ml
7) N-EICOSANE	12.508	104705	0.661 ug/ml
10) N-TETRACOSANE	14.822	417463	2.668 ug/ml
11) N-HEXACOSANE	15.876	128995	0.828 ug/ml
12) N-OCTACOSANE	16.825	307669	1.983 ug/ml
13) N-TRIACONTANE	17.716	246896	1.591 ug/ml
14) N-DOTRIACONTANE	18.550	242729	1.565 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103018\
Data File : FF002511.D
Signal(s) : FID2B.ch
Acq On : 30 Oct 2018 18:20
Operator : AJ\SJ
Sample : J5724-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 31 00:40:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

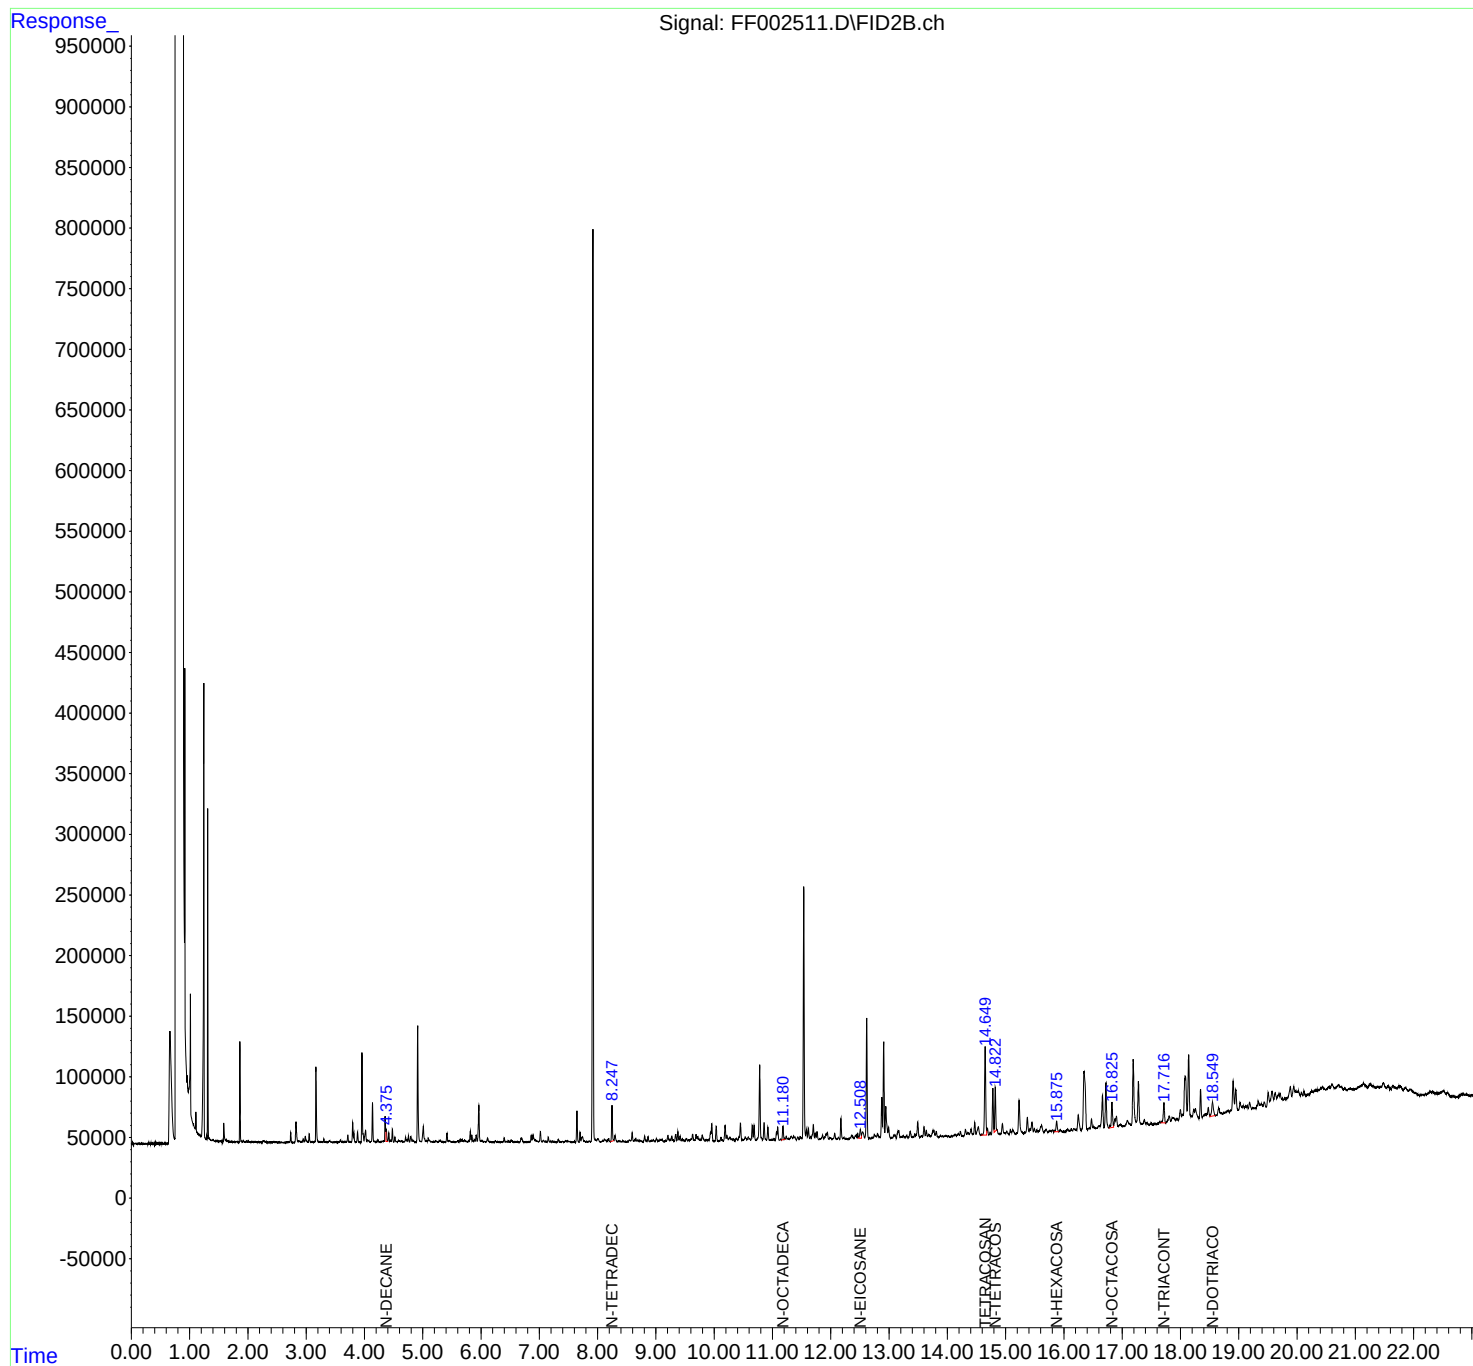

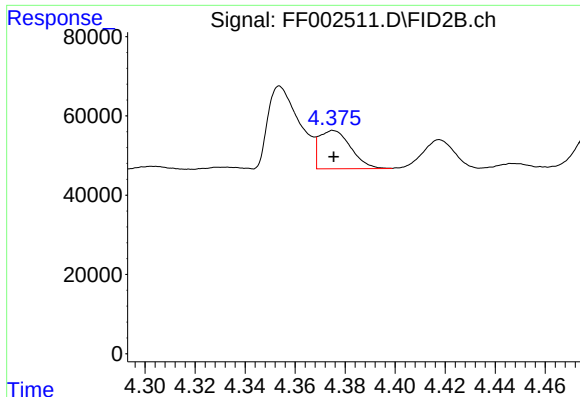


#2 N-DECANE

R.T.: 4.375 min
Delta R.T.: 0.000 min
Response: 85208
Conc: 0.56 ug/ml

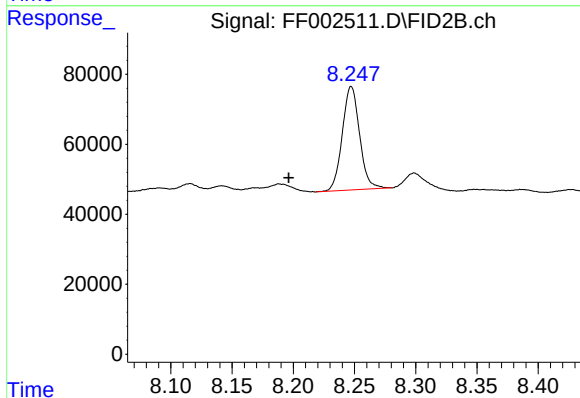


#4 N-TETRADECANE

R.T.: 8.247 min
Delta R.T.: 0.051 min
Response: 290740
Conc: 1.86 ug/ml

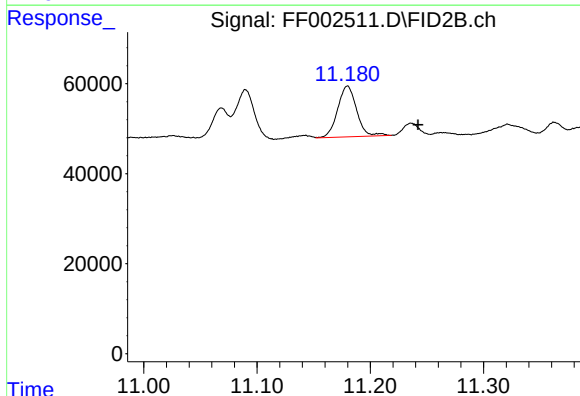


#6 N-OCTADECANE

R.T.: 11.180 min
Delta R.T.: -0.062 min
Response: 131232
Conc: 0.83 ug/ml

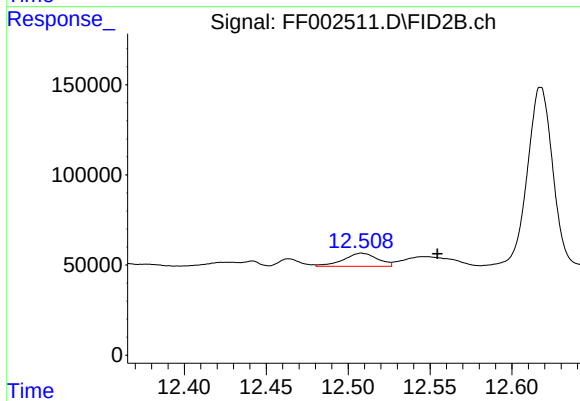


#7 N-EICOSANE

R.T.: 12.508 min
Delta R.T.: -0.046 min
Response: 104705
Conc: 0.66 ug/ml

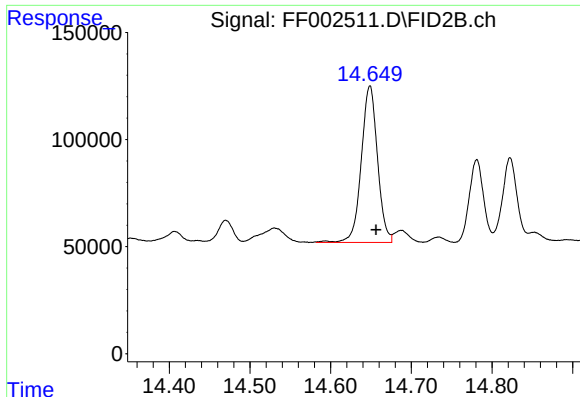


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.649 min
Delta R.T.: -0.008 min
Response: 1021117
Conc: 7.35 ug/ml

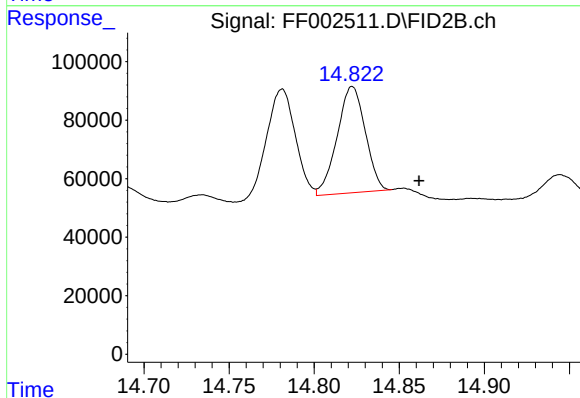


#10 N-TETRACOSANE

R.T.: 14.822 min
Delta R.T.: -0.039 min
Response: 417463
Conc: 2.67 ug/ml

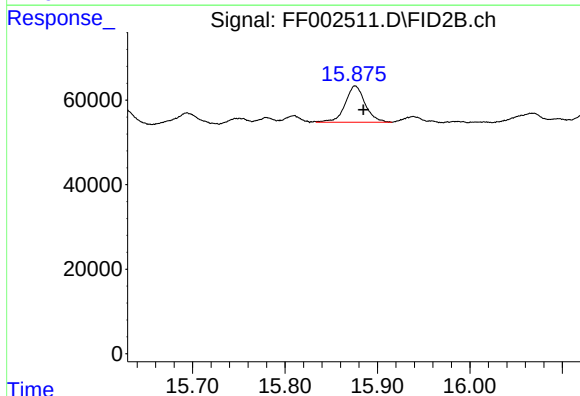


#11 N-HEXACOSANE

R.T.: 15.876 min
Delta R.T.: -0.009 min
Response: 128995
Conc: 0.83 ug/ml

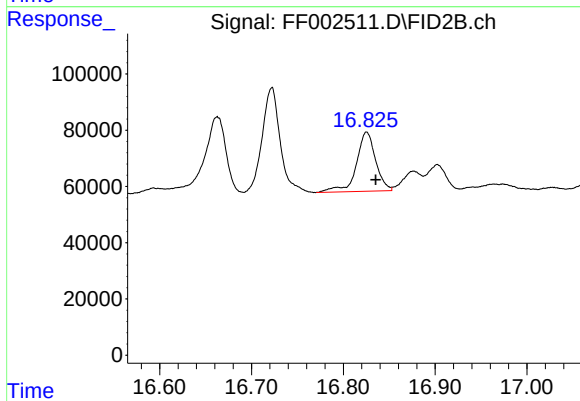


#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.010 min
Response: 307669
Conc: 1.98 ug/ml

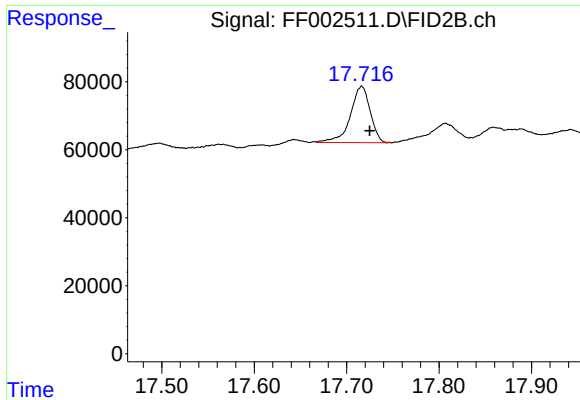

#13 N-TRIACONTANE

R.T.: 17.716 min
Delta R.T.: -0.009 min
Response: 246896
Conc: 1.59 ug/ml

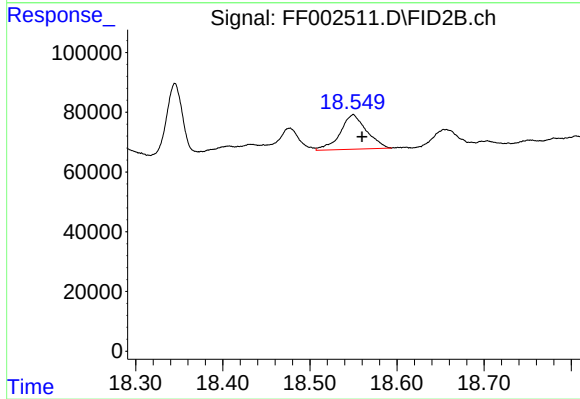

#14 N-DOTRIACONTANE

R.T.: 18.550 min
Delta R.T.: -0.010 min
Response: 242729
Conc: 1.57 ug/ml