

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE103119\  
 Data File : FE030743.D  
 Signal(s) : FID1B.CH  
 Acq On : 31 Oct 2019 15:51  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 I.BLK

Integration File: autoint1.e  
 Quant Time: Nov 01 02:22:10 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE103019.M  
 Quant Title :  
 QLast Update : Thu Oct 31 08:47:02 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.652 | 6961021  | 22.398 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 17.708 | 215898   | 0.650 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.540 | 272650   | 0.854 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE103119\  
Data File : FE030743.D  
Signal(s) : FID1B.CH  
Acq On : 31 Oct 2019 15:51  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Nov 01 02:22:10 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE103019.M  
Quant Title :  
QLast Update : Thu Oct 31 08:47:02 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

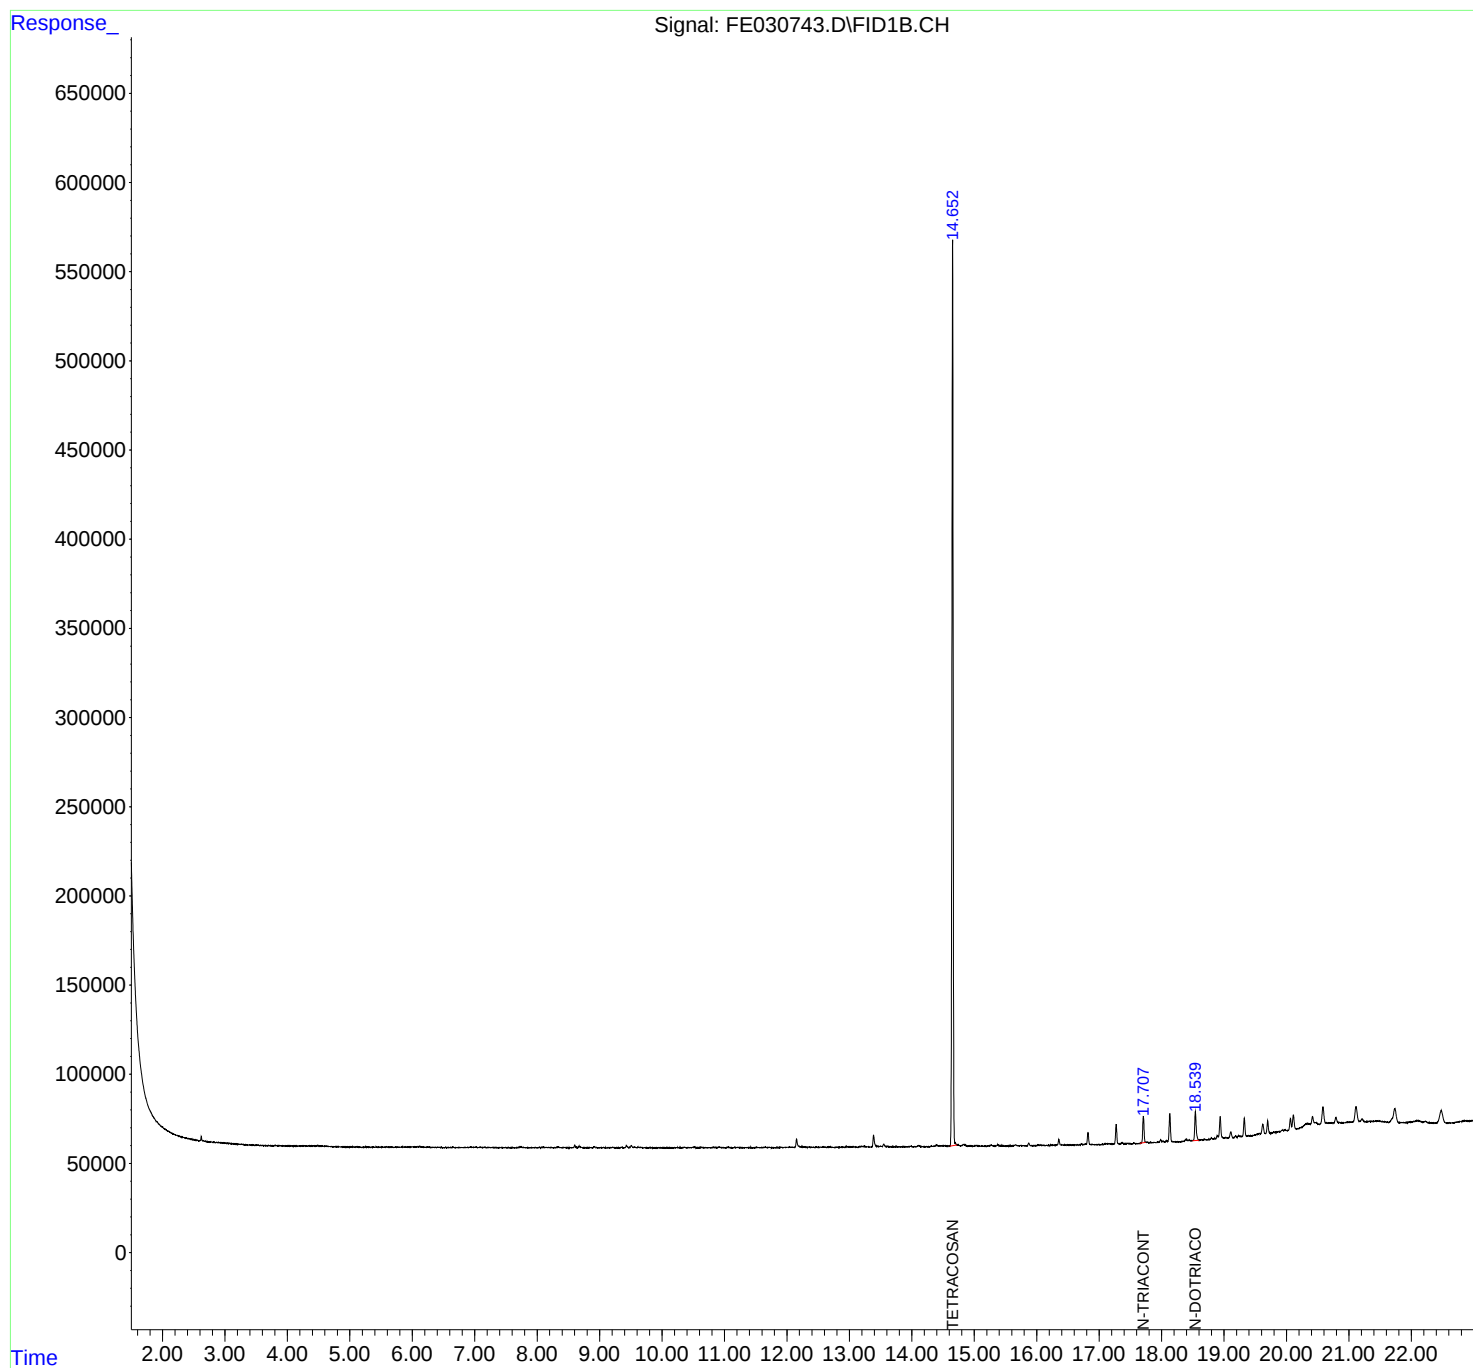


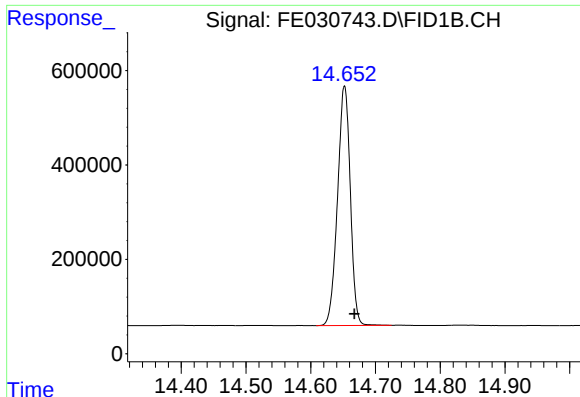

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.652 min  
Delta R.T.: -0.015 min  
Response: 6961021  
Conc: 22.40 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

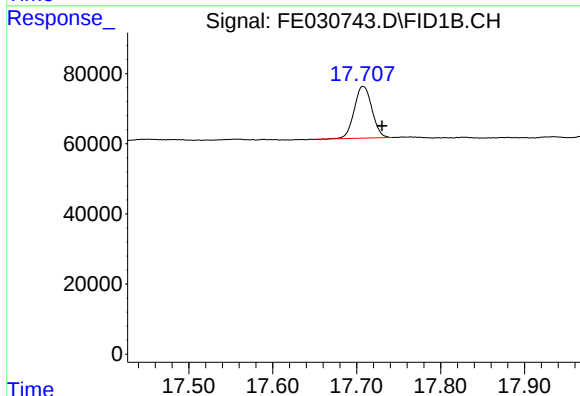

#13 N-TRIACONTANE

R.T.: 17.708 min  
Delta R.T.: -0.022 min  
Response: 215898  
Conc: 0.65 ug/ml

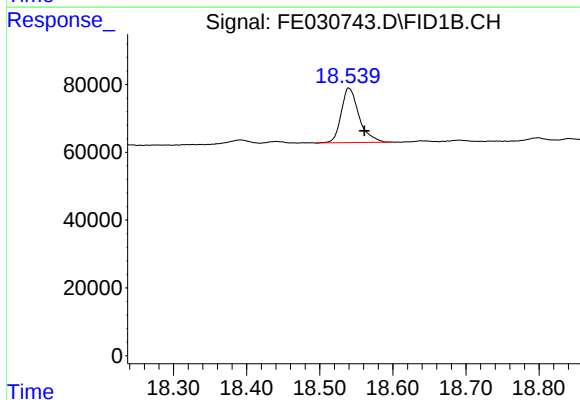

#14 N-DOTRIACONTANE

R.T.: 18.540 min  
Delta R.T.: -0.021 min  
Response: 272650  
Conc: 0.85 ug/ml