

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE103119\  
 Data File : FE030737.D  
 Signal(s) : FID1B.CH  
 Acq On : 31 Oct 2019 12:17  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 RT MARKER

Integration File: autoint1.e  
 Quant Time: Nov 01 02:21:06 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE103019.M  
 Quant Title :  
 QLast Update : Thu Oct 31 08:47:02 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.406  | 9306784  | 24.459 ug/ml |
| 12) N-OCTACOSANE            | 16.826 | 8851088  | 25.961 ug/ml |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE103119\  
Data File : FE030737.D  
Signal(s) : FID1B.CH  
Acq On : 31 Oct 2019 12:17  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Nov 01 02:21:06 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE103019.M  
Quant Title :  
QLast Update : Thu Oct 31 08:47:02 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

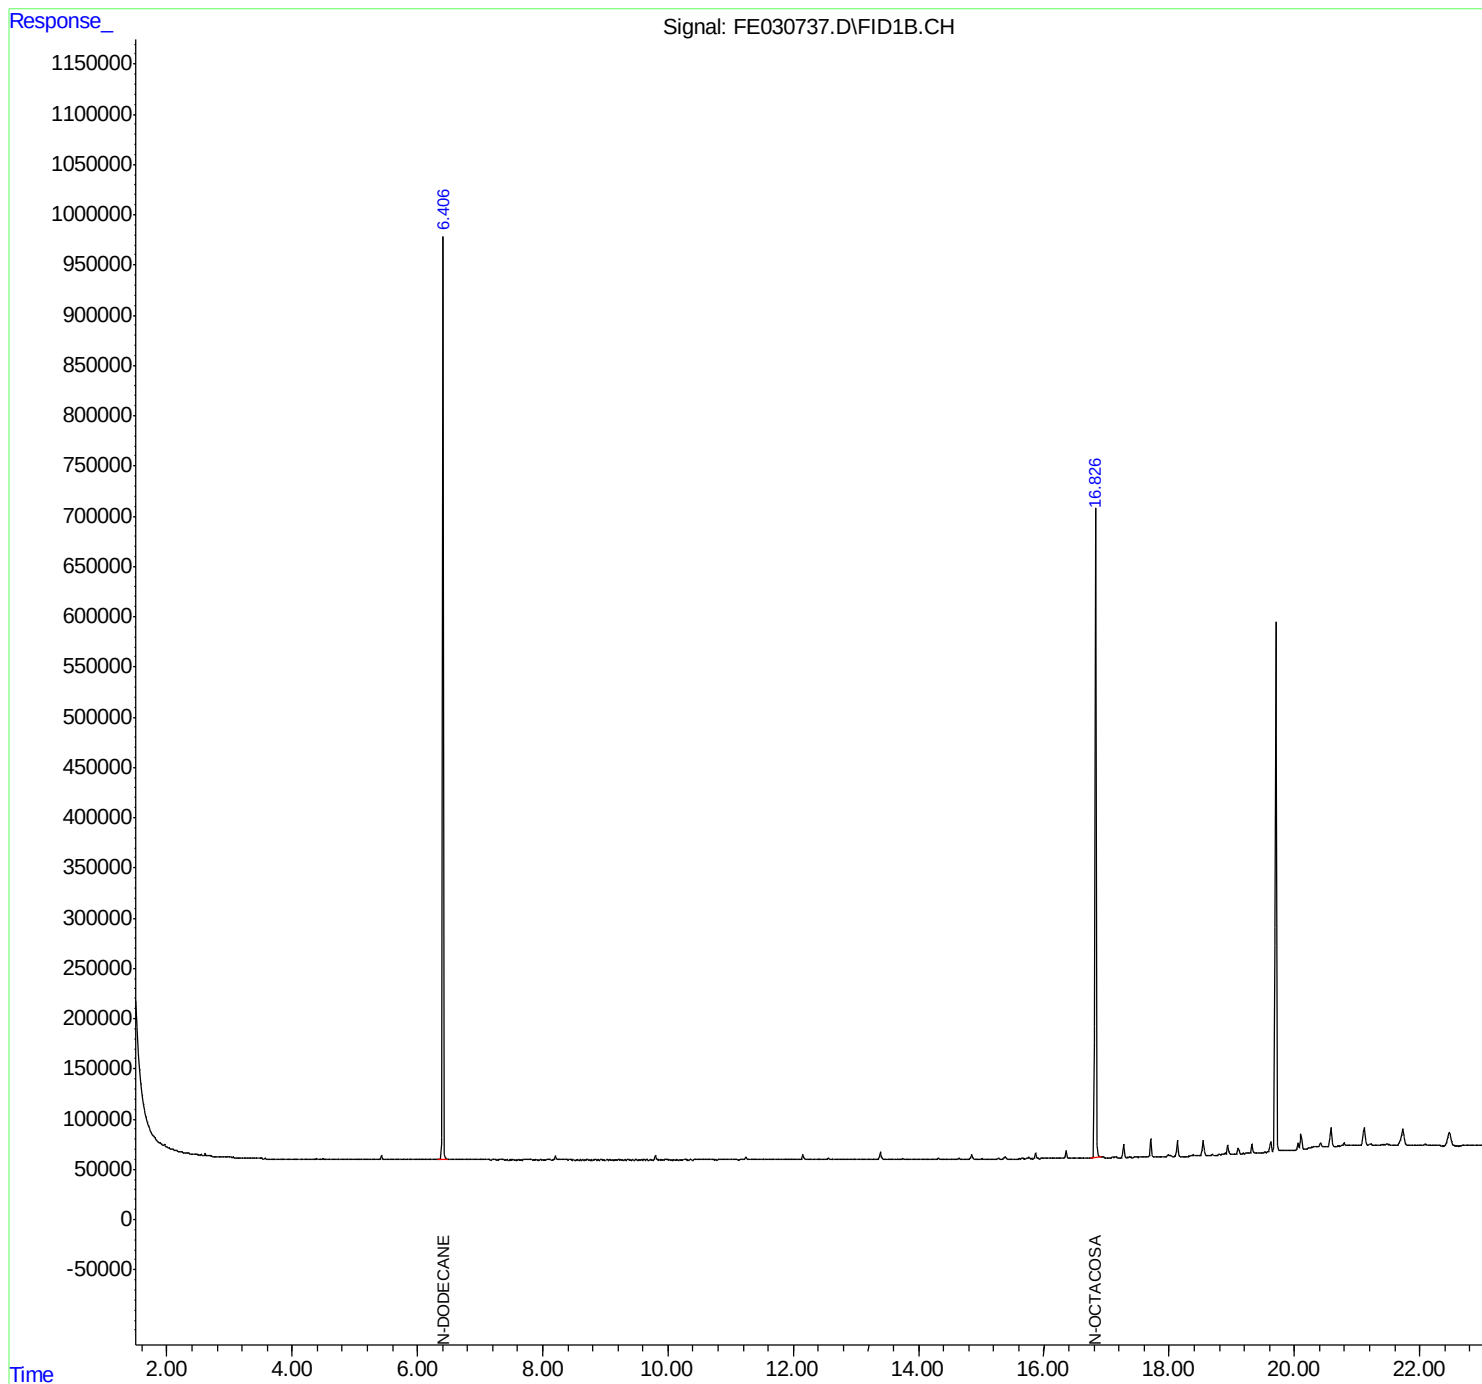


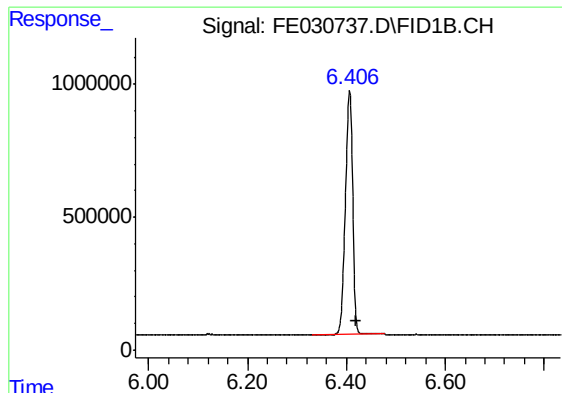

#3 N-DODECANE


R.T.: 6.406 min  
Delta R.T.: -0.013 min  
Response: 9306784  
Conc: 24.46 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
RT MARKER

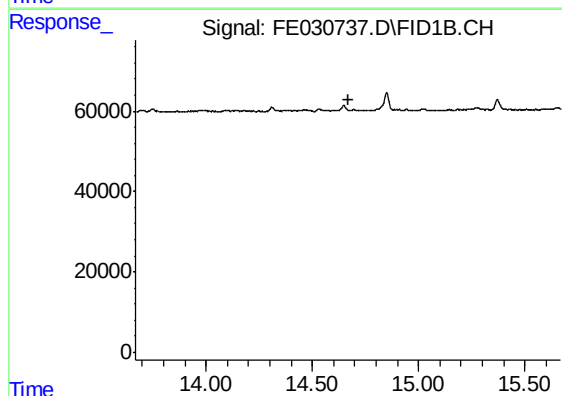

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.667 min  
Response: 0  
Conc: N.D.

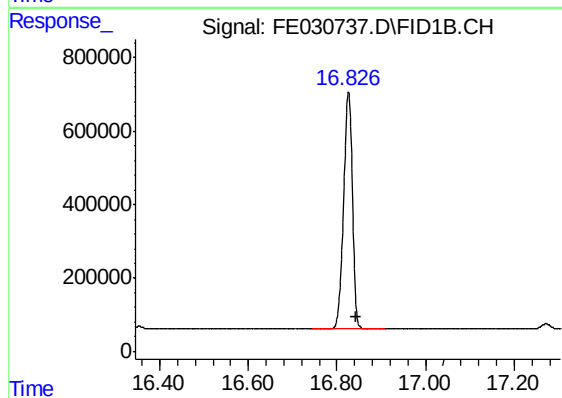

#12 N-OCTACOSANE

R.T.: 16.826 min  
Delta R.T.: -0.017 min  
Response: 8851088  
Conc: 25.96 ug/ml