

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE103125AL\
Data File : FE056600.D
Signal(s) : FID1B.ch
Acq On : 31 Oct 2025 08:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 31 23:10:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 12:50:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.977	130499	0.664 ug/ml
19) T	n-Tetratriacontane (C34)	19.763	294145	1.704 ug/ml
20) T	n-Hexatriacontane (C36)	20.505	1032142	7.135 ug/ml
21) T	n-Octatriacontane (C38)	21.262	1912866	15.198 ug/ml
22) T	n-Tetracontane (C40)	22.208	1336679	11.562 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE103125AL\
Data File : FE056600.D
Signal(s) : FID1B.ch
Acq On : 31 Oct 2025 08:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 31 23:10:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 12:50:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

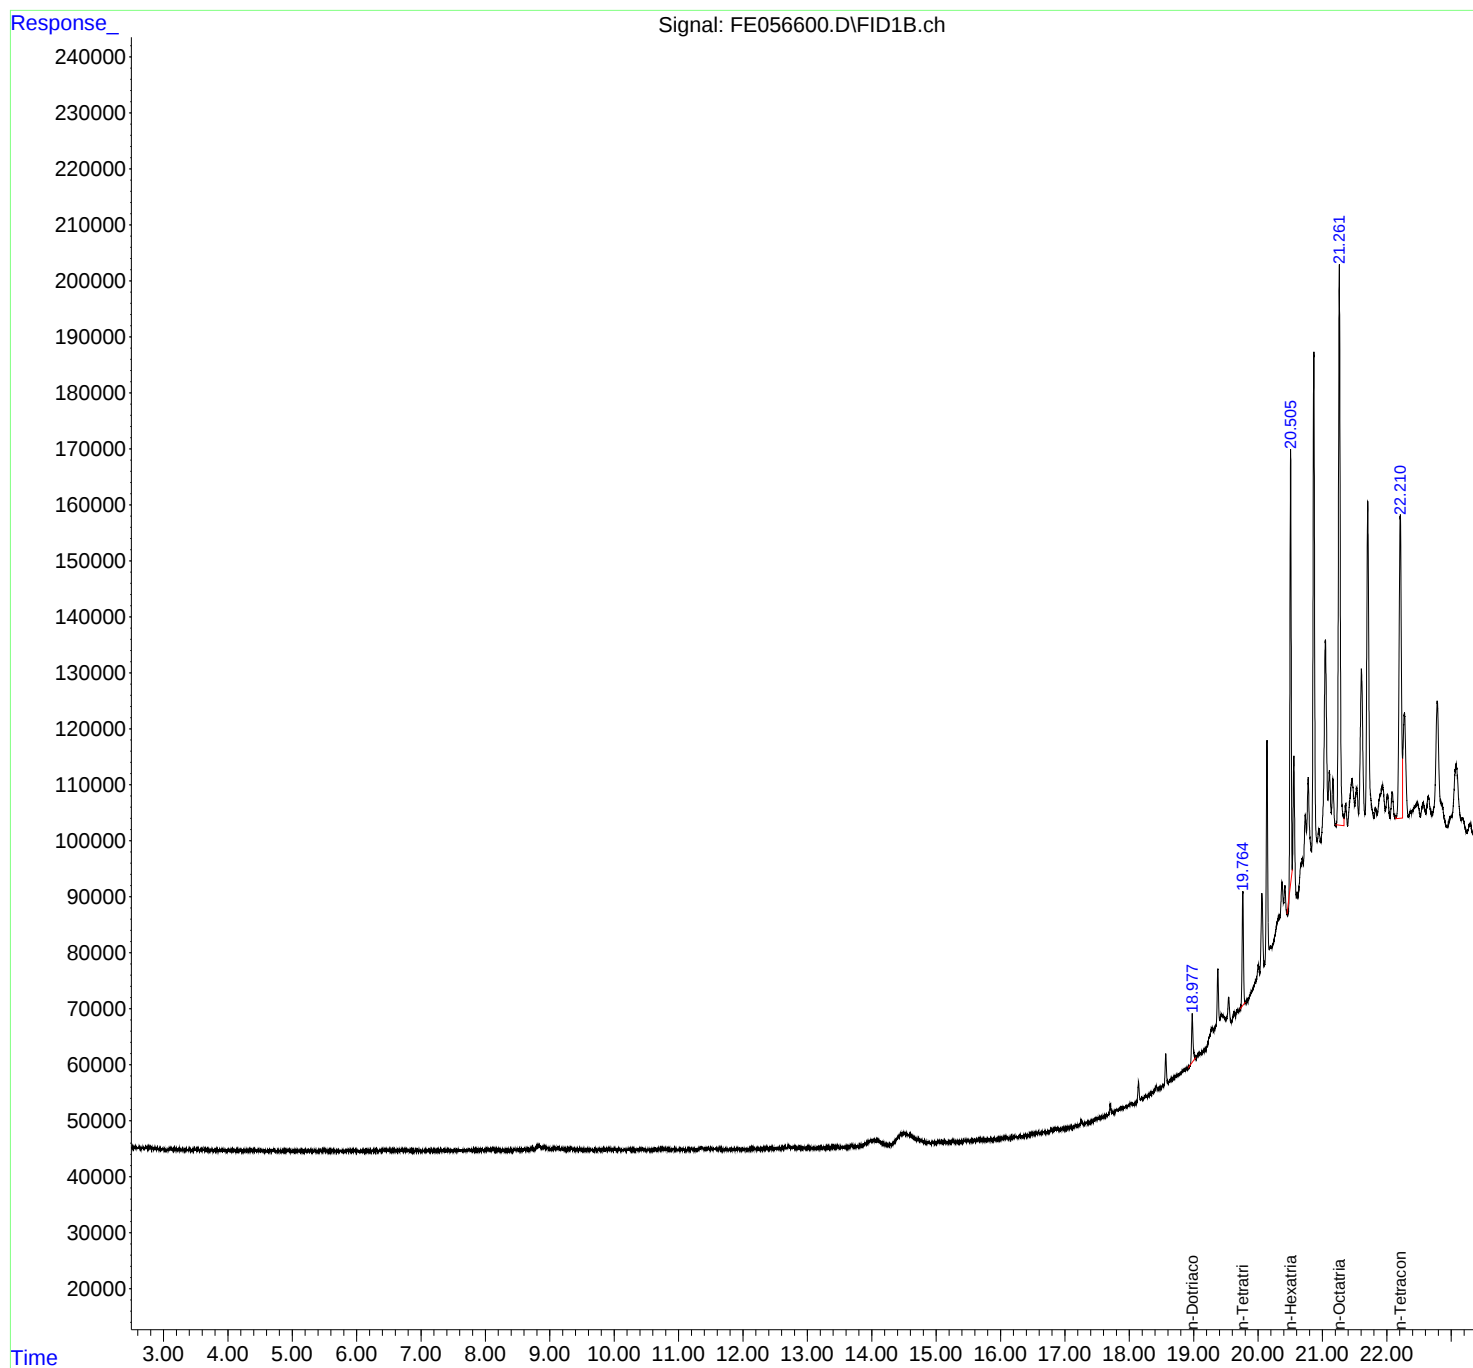


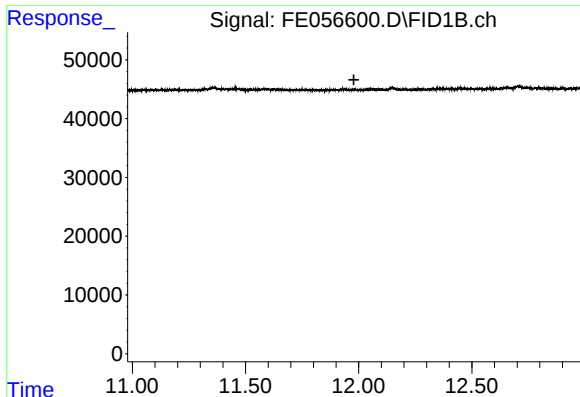

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.979 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

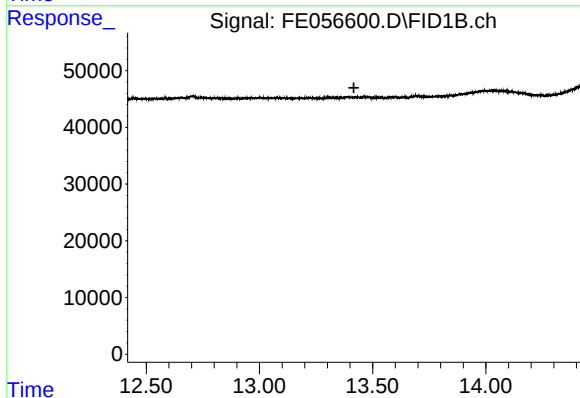


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.417 min
Response: 0
Conc: N.D.

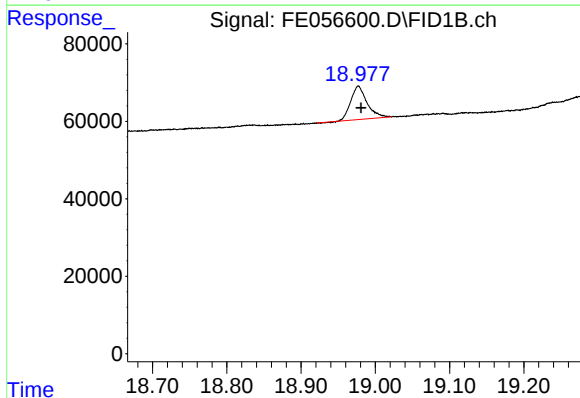


#18 n-Dotriacontane (C32)

R.T.: 18.977 min
Delta R.T.: -0.003 min
Response: 130499
Conc: 0.66 ug/ml

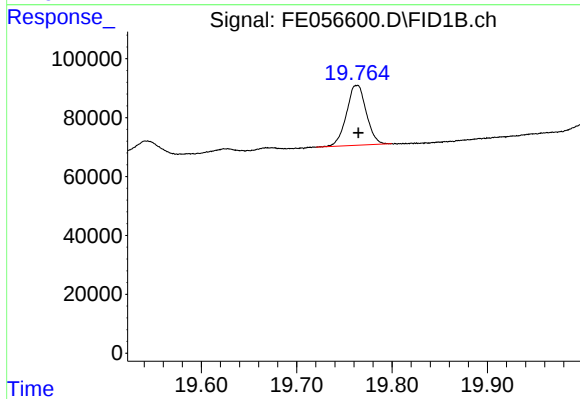

#19 n-Tetratriacontane (C34)


R.T.: 19.763 min
Delta R.T.: -0.002 min
Response: 294145
Conc: 1.70 ug/ml

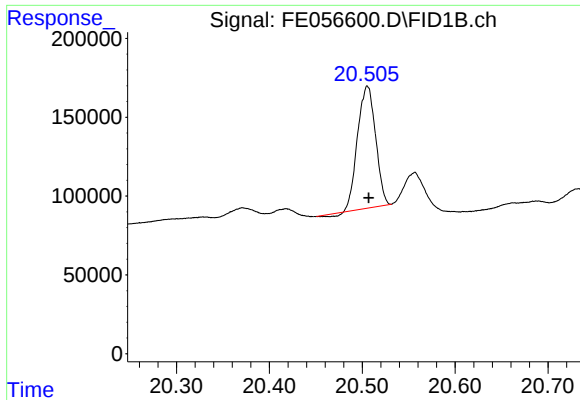

#20 n-Hexatriacontane (C36)


R.T.: 20.505 min
Delta R.T.: -0.002 min
Response: 1032142
Conc: 7.14 ug/ml

Instrument :
FID_E
ClientSampleId :

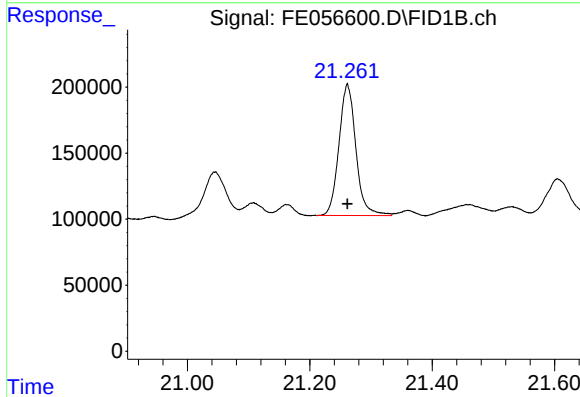

#21 n-Octatriacontane (C38)

R.T.: 21.262 min
Delta R.T.: 0.000 min
Response: 1912866
Conc: 15.20 ug/ml

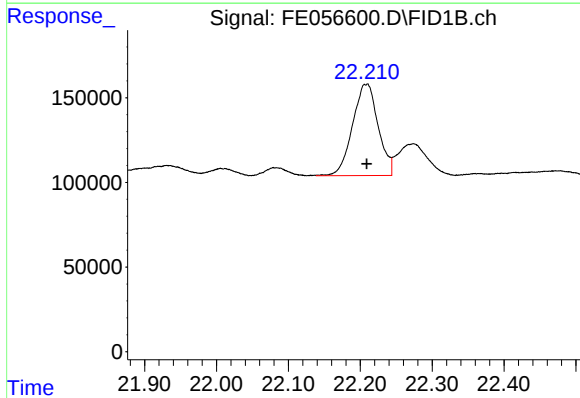

#22 n-Tetracontane (C40)

R.T.: 22.208 min
Delta R.T.: 0.000 min
Response: 1336679
Conc: 11.56 ug/ml