

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110222AL\  
 Data File : FE038520.D  
 Signal(s) : FID1B.ch  
 Acq On : 03 Nov 2022 00:36  
 Operator : YP\AJ  
 Sample : N5396-16  
 Misc :  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 TP-H

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 11/03/2022  
 Supervised By :Ankita Jodhani 11/03/2022

Integration File: autoint1.e  
 Quant Time: Nov 03 04:25:53 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102522.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Oct 26 04:49:29 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 11.965 | 4871523    | 28.311 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 56.62%        |
| 12) S 1-chlorooctadecane (S... | 13.398 | 3917248    | 28.614 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 57.23%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110222AL\  
Data File : FE038520.D  
Signal(s) : FID1B.ch  
Acq On : 03 Nov 2022 00:36  
Operator : YP\AJ  
Sample : N5396-16  
Misc :  
ALS Vial : 27 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
TP-H


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/03/2022  
Supervised By :Ankita Jodhani 11/03/2022

Integration File: autoint1.e  
Quant Time: Nov 03 04:25:53 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102522.M  
Quant Title : GC Extractables  
QLast Update : Wed Oct 26 04:49:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

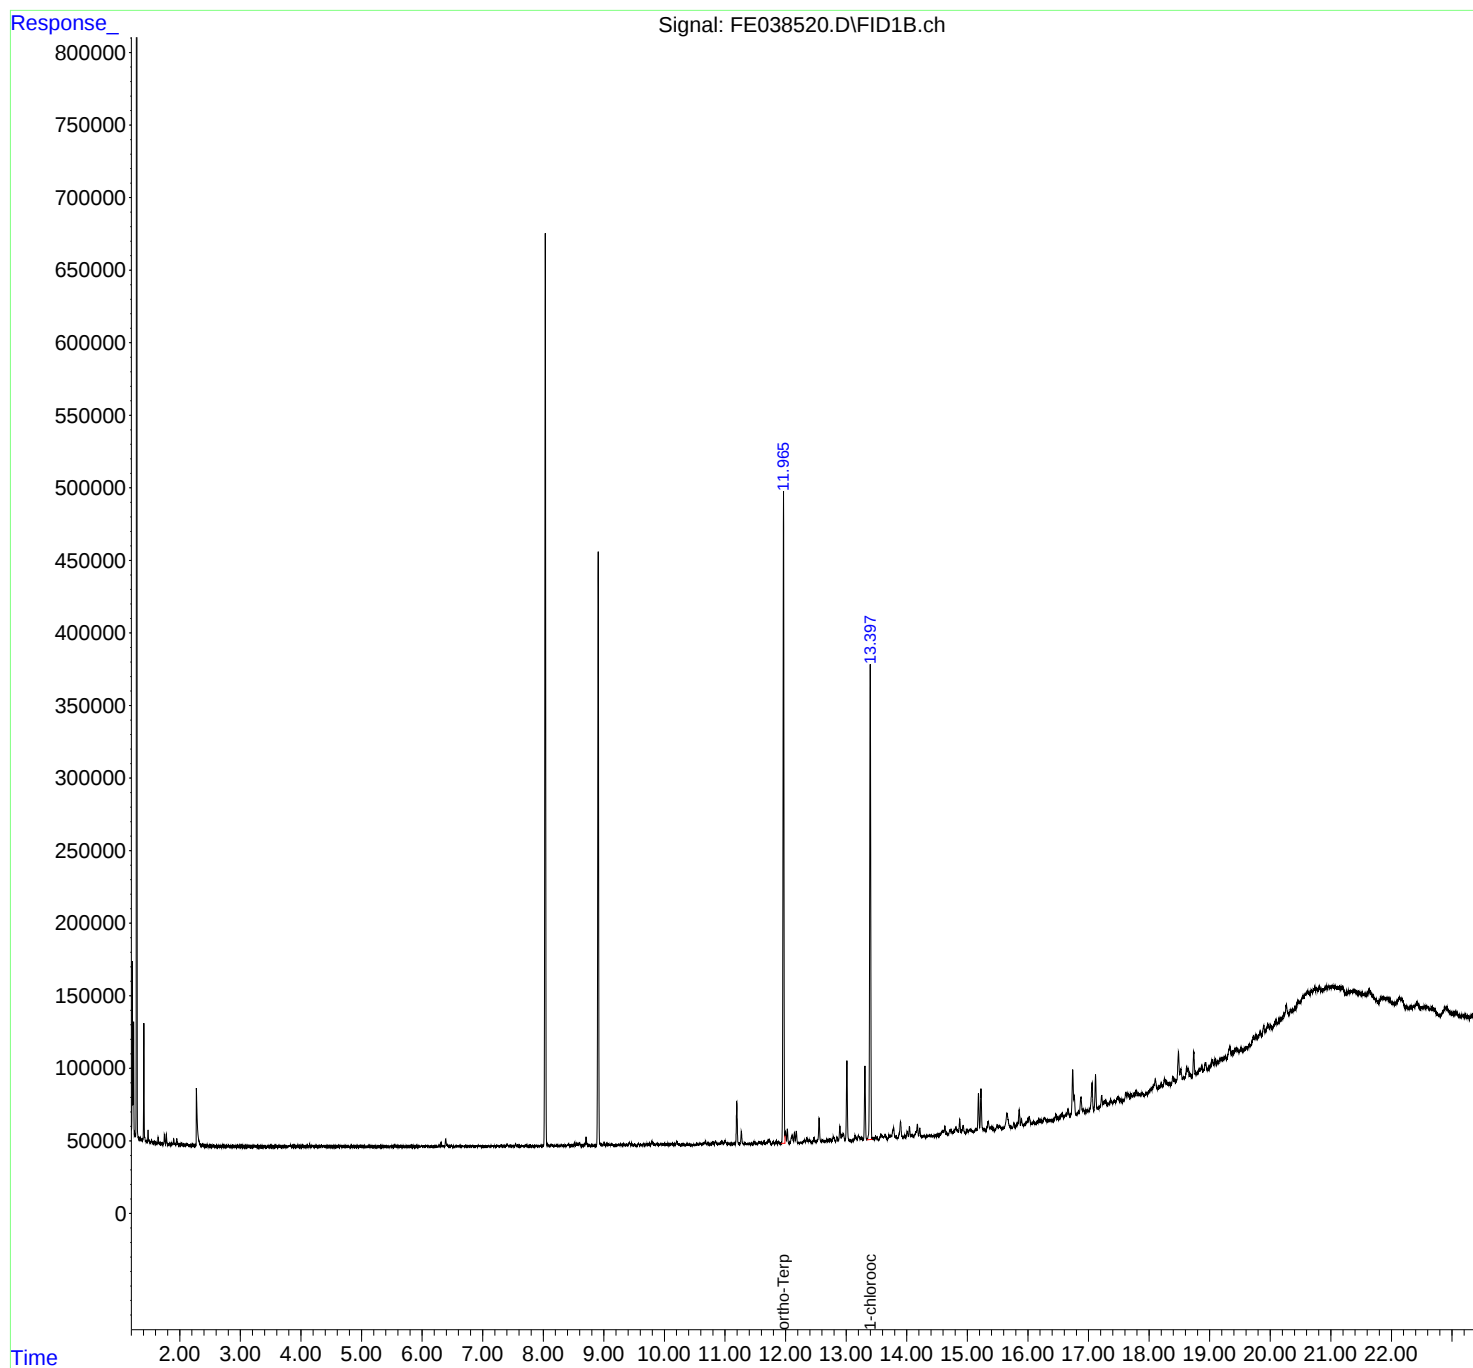

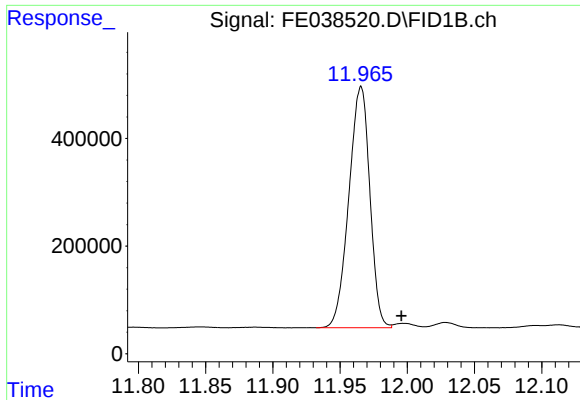


#9 ortho-Terphenyl (SURR)

R.T.: 11.965 min  
Delta R.T.: -0.030 min  
Response: 4871523  
Conc: 28.31 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
TP-H

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/03/2022  
Supervised By :Ankita Jodhani 11/03/2022

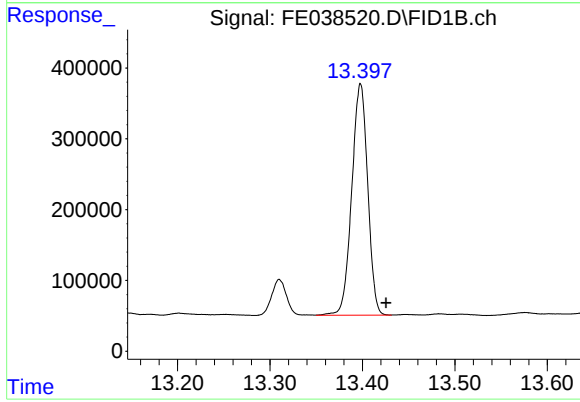

#12 1-chlorooctadecane (SURR)

R.T.: 13.398 min  
Delta R.T.: -0.028 min  
Response: 3917248  
Conc: 28.61 ug/ml