

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110320\
Data File : FE033100.D
Signal(s) : FID1B.CH
Acq On : 03 Nov 2020 6:58
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 04 00:14:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) N-TETRACONTANE	21.727	406347	2.480 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110320\
Data File : FE033100.D
Signal(s) : FID1B.CH
Acq On : 03 Nov 2020 6:58
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 04 00:14:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

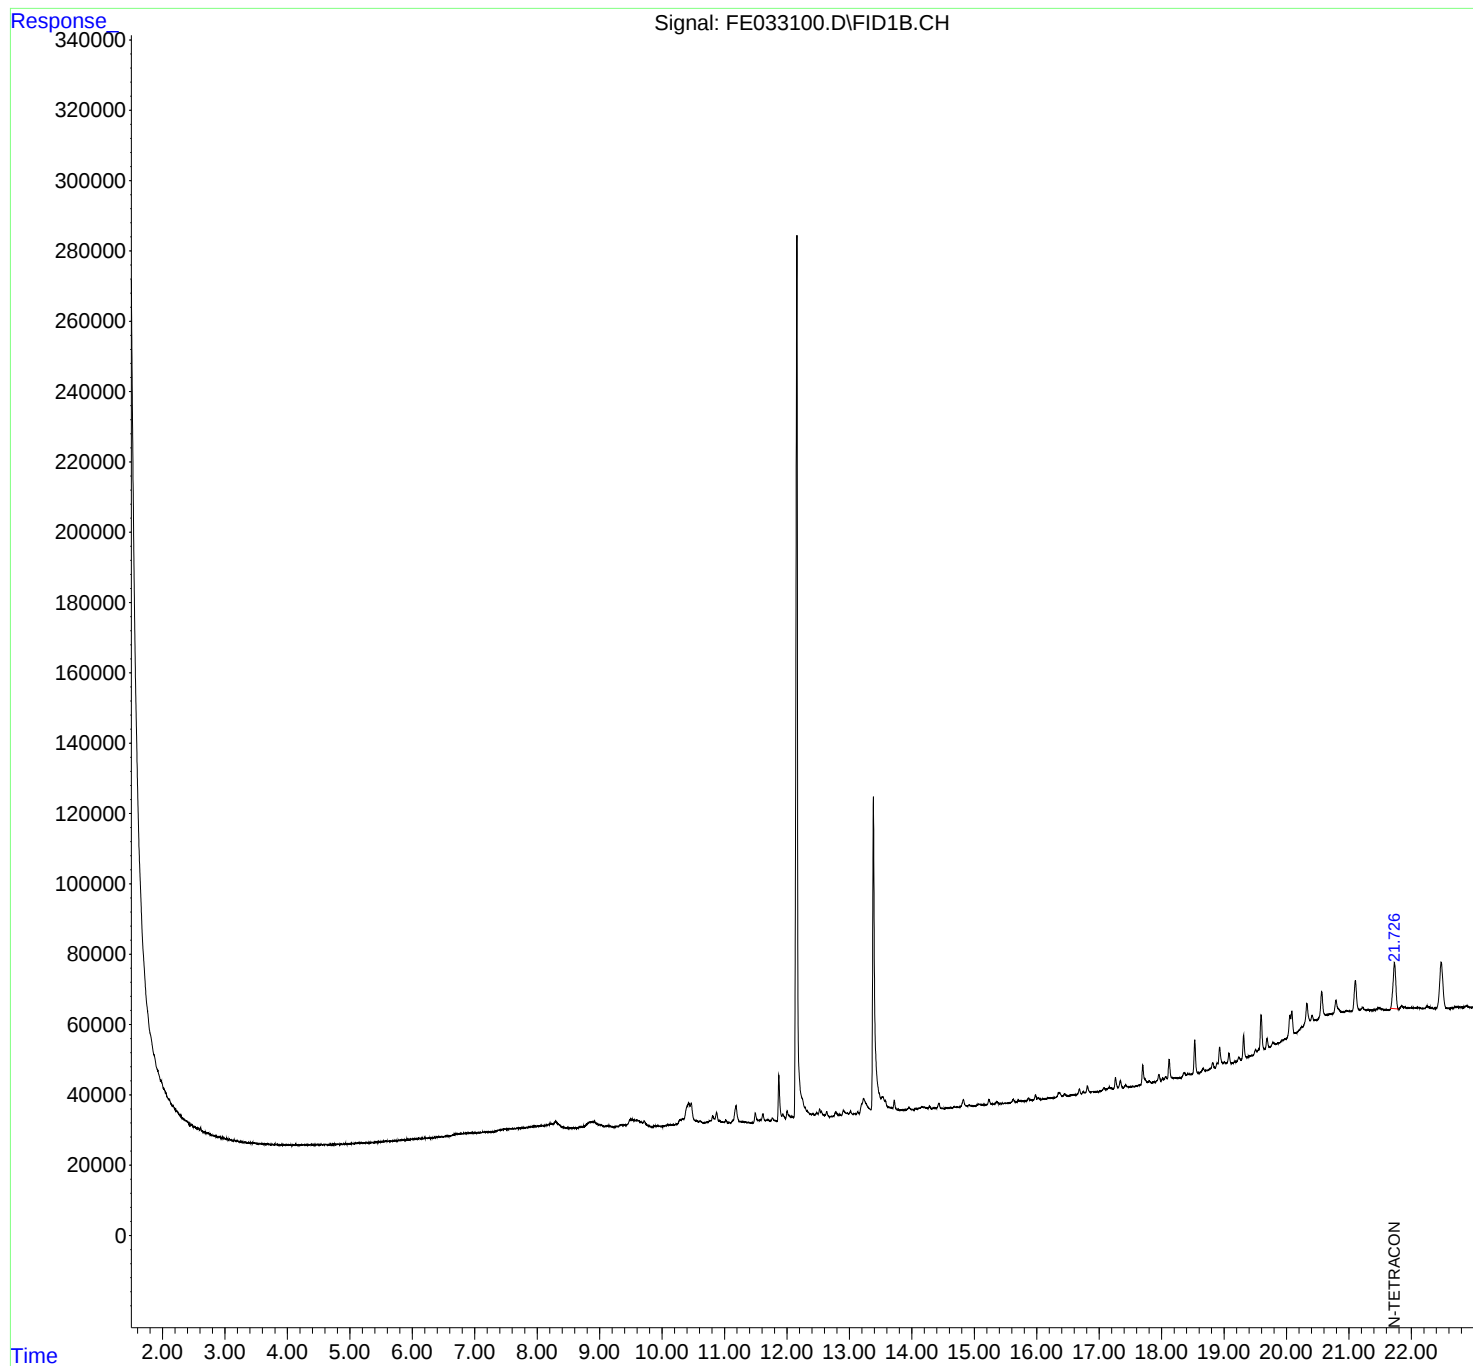


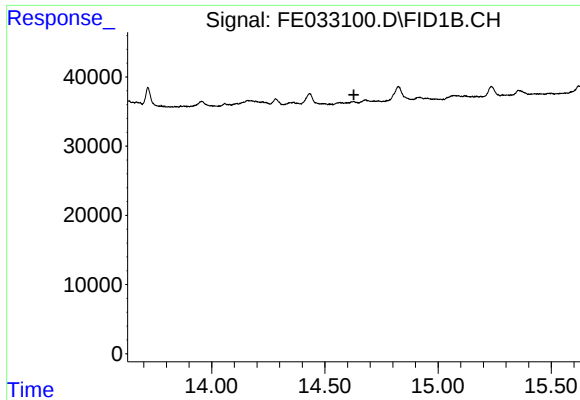

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.628 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

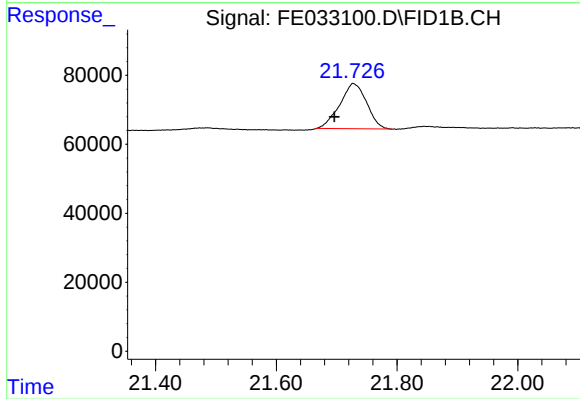

#18 N-TETRACONTANE

R.T.: 21.727 min
Delta R.T.: 0.031 min
Response: 406347
Conc: 2.48 ug/ml