

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110323AL\
 Data File : FE045168.D
 Signal(s) : FID1B.ch
 Acq On : 03 Nov 2023 05:32
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 03 23:02:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 101223.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 12 06:15:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.877	169655	1.016 ug/ml
11) T n-Heneicosane (C21)	13.494	310747	1.906 ug/ml
13) T n-Docosane (C22)	14.085	309517	1.935 ug/ml
14) T n-Tetracosane (C24)	15.194	203741	1.313 ug/ml
15) T n-Hexacosane (C26)	16.217	187177	1.247 ug/ml
16) T n-Octacosane (C28)	17.171	192074	1.308 ug/ml
17) T n-Tricontane (C30)	18.060	226300	1.522 ug/ml
18) T n-Dotriacontane (C32)	18.897	297137	1.980 ug/ml
19) T n-Tetratriacontane (C34)	19.680	313040	2.103 ug/ml
20) T n-Hexatriacontane (C36)	20.421	88594	0.576 ug/ml
22) T n-Tetracontane (C40)	22.074	90309	0.540 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110323AL\
Data File : FE045168.D
Signal(s) : FID1B.ch
Acq On : 03 Nov 2023 05:32
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 23:02:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 101223.M
Quant Title : GC Extractables
QLast Update : Thu Oct 12 06:15:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

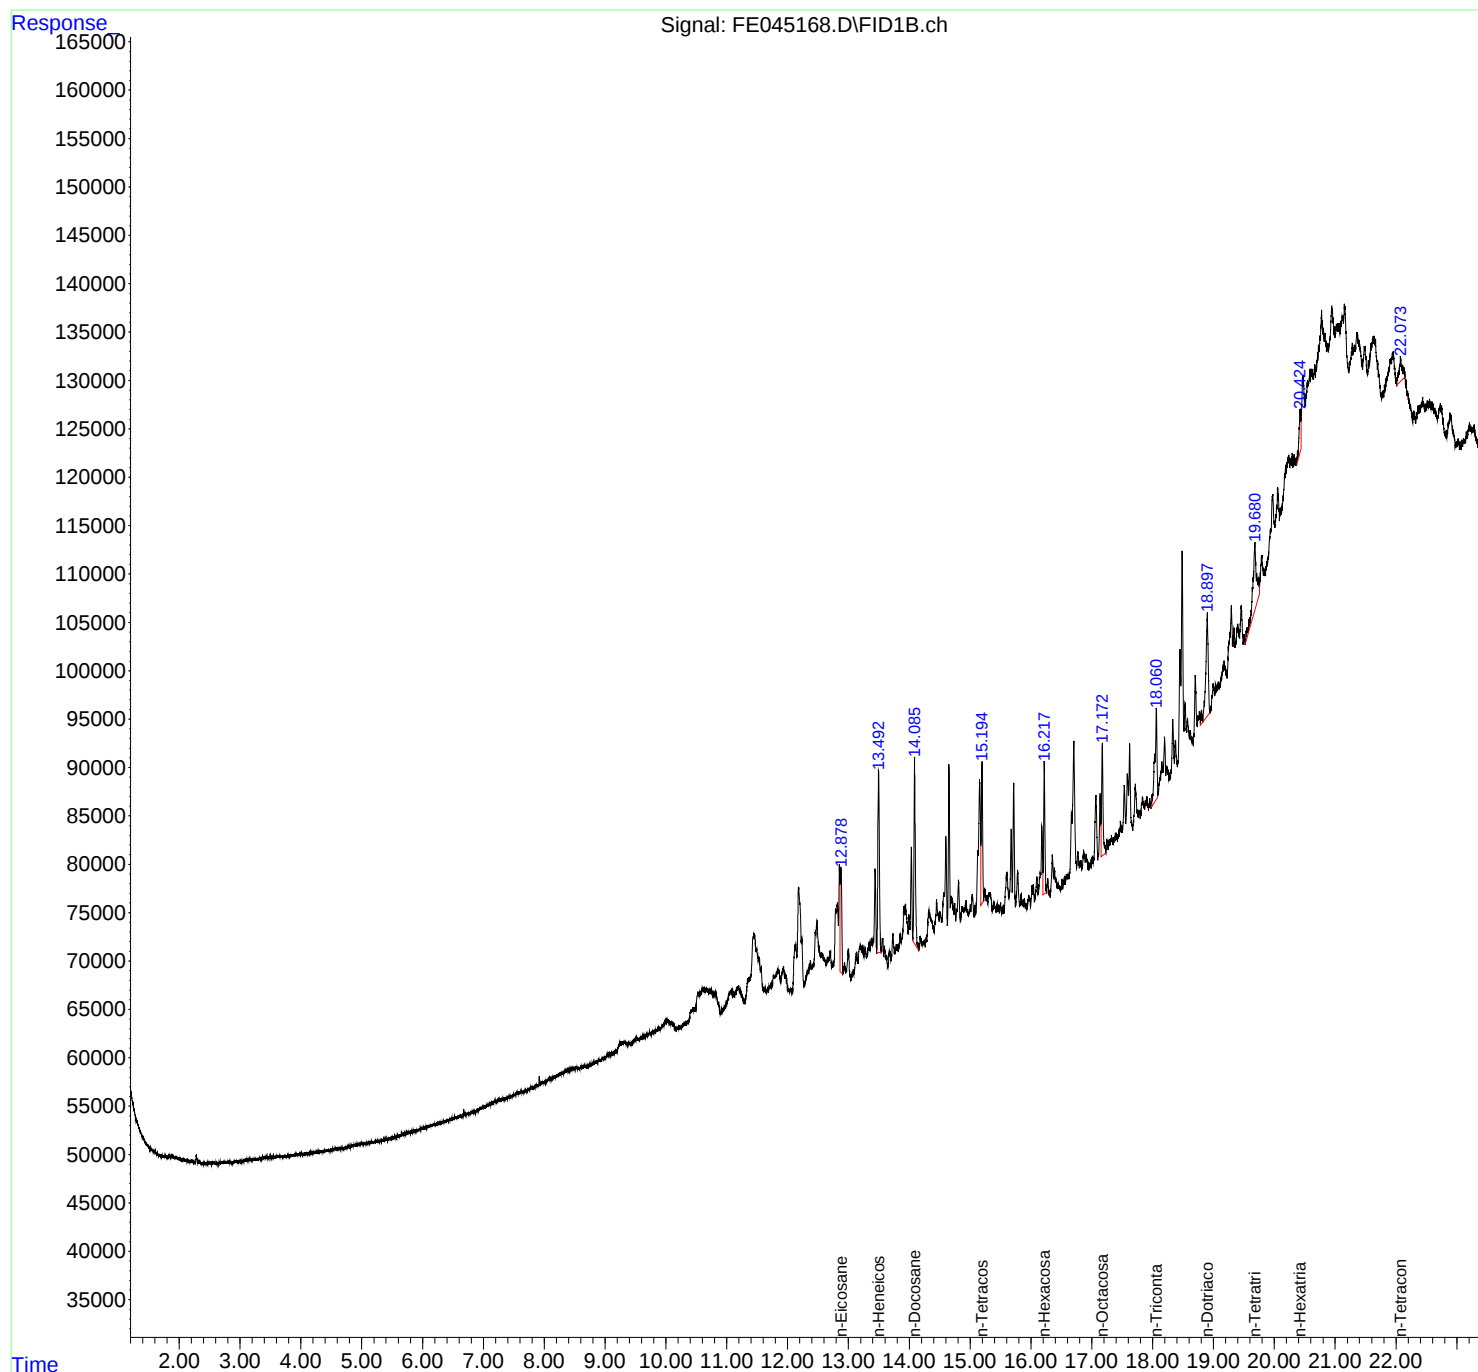


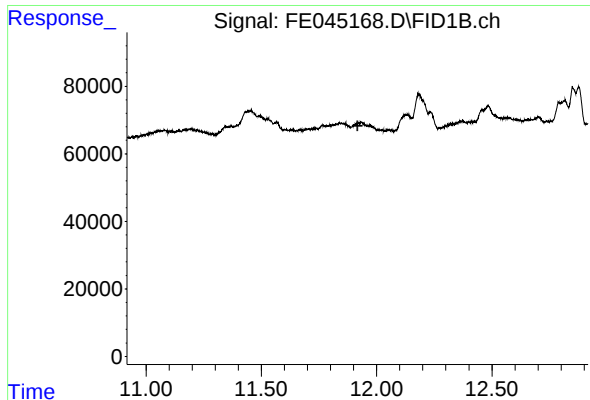

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.917 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

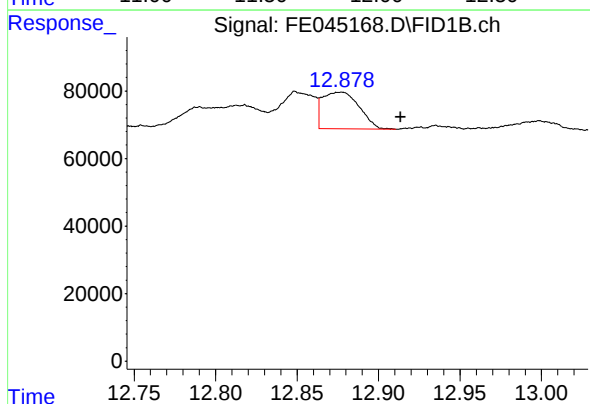


#10 n-Eicosane (C20)

R.T.: 12.877 min
Delta R.T.: -0.036 min
Response: 169655
Conc: 1.02 ug/ml

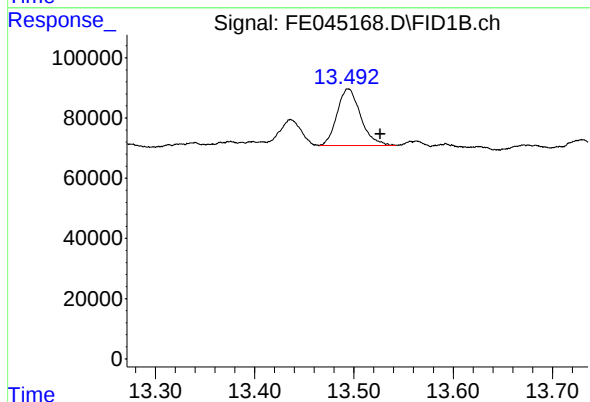


#11 n-Heneicosane (C21)

R.T.: 13.494 min
Delta R.T.: -0.032 min
Response: 310747
Conc: 1.91 ug/ml

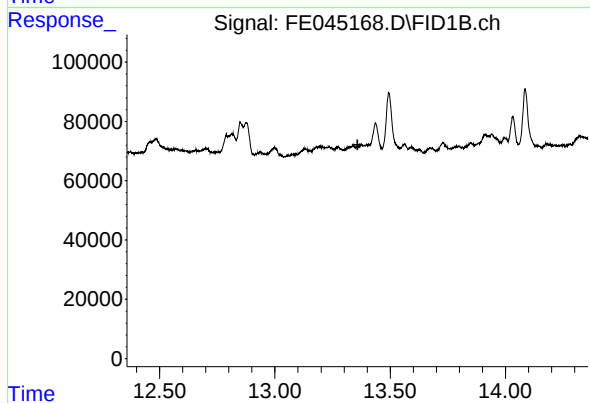

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.358 min
Response: 0
Conc: N.D.

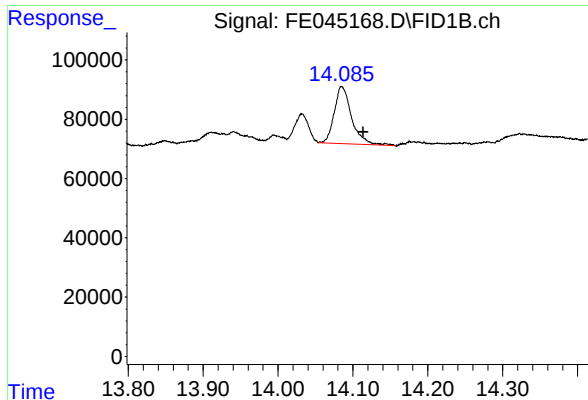

#13 n-Docosane (C22)


R.T.: 14.085 min
Delta R.T.: -0.029 min
Response: 309517
Conc: 1.94 ug/ml

Instrument :
FID_E
ClientSampleId :

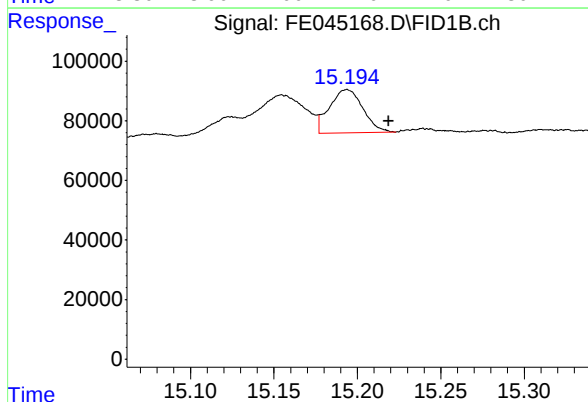


#14 n-Tetracosane (C24)

R.T.: 15.194 min
Delta R.T.: -0.025 min
Response: 203741
Conc: 1.31 ug/ml

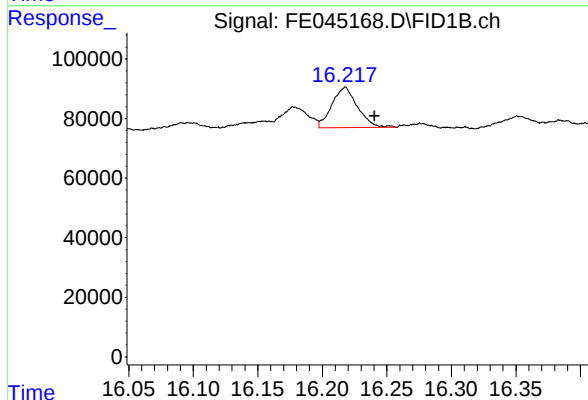


#15 n-Hexacosane (C26)

R.T.: 16.217 min
Delta R.T.: -0.023 min
Response: 187177
Conc: 1.25 ug/ml

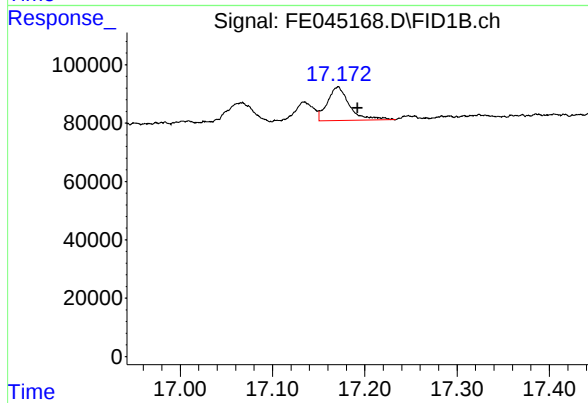

#16 n-Octacosane (C28)


R.T.: 17.171 min
Delta R.T.: -0.022 min
Response: 192074
Conc: 1.31 ug/ml

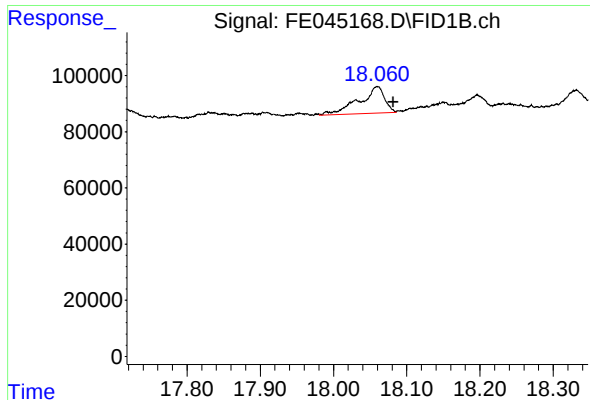

#17 n-Tricontane (C30)


R.T.: 18.060 min
Delta R.T.: -0.022 min
Response: 226300
Conc: 1.52 ug/ml

Instrument :
FID_E
ClientSampleId :

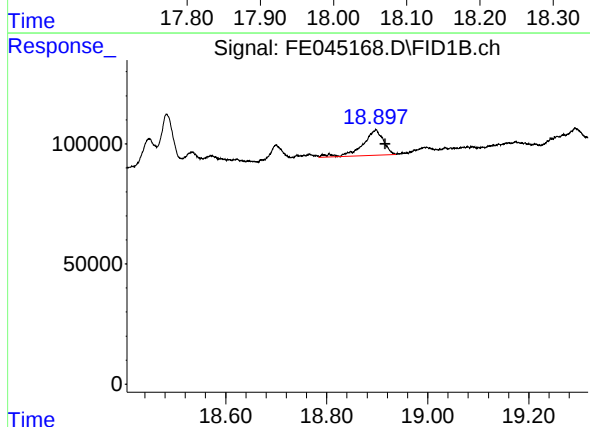


#18 n-Dotriacontane (C32)

R.T.: 18.897 min
Delta R.T.: -0.019 min
Response: 297137
Conc: 1.98 ug/ml

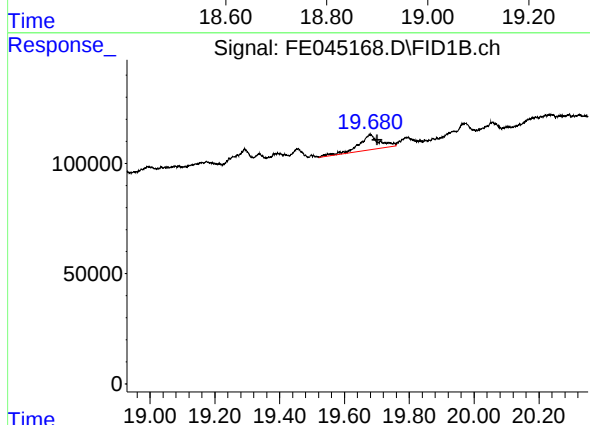


#19 n-Tetratriacontane (C34)

R.T.: 19.680 min
Delta R.T.: -0.021 min
Response: 313040
Conc: 2.10 ug/ml

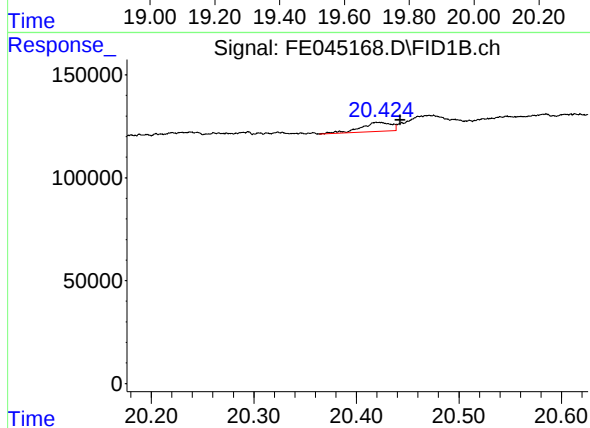

#20 n-Hexatriacontane (C36)

R.T.: 20.421 min
Delta R.T.: -0.021 min
Response: 88594
Conc: 0.58 ug/ml

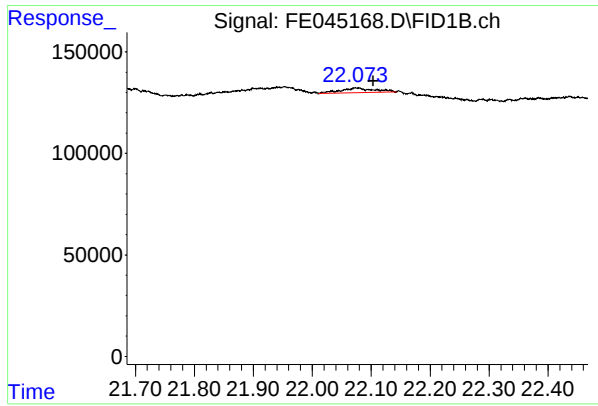

#22 n-Tetracontane (C40)

R.T.: 22.074 min

Delta R.T.: -0.029 min

Response: 90309

Conc: 0.54 ug/ml

Instrument :

FID_E

ClientSampleId :