

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110325\
Data File : FB032274.D
Signal(s) : FID2B.CH
Acq On : 3 Nov 2025 11:58
Operator : YP/AJ
Sample : VBF1103S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
VBF1103S1

Integration File: Calibrat.e
Quant Time: Nov 04 04:52:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	412678	20.346 ng/ml
Target Compounds			
6) t Toluene	10.616	5579	0.156 ng/ml
8) t m-Xylene	13.201	6329	0.190 ng/ml
9) t O-Xylene	13.920	6020	0.187 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	12430	0.449 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110325\
Data File : FB032274.D
Signal(s) : FID2B.CH
Acq On : 3 Nov 2025 11:58
Operator : YP/AJ
Sample : VBF1103S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
VBF1103S1

Integration File: Calibrat.e
Quant Time: Nov 04 04:52:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

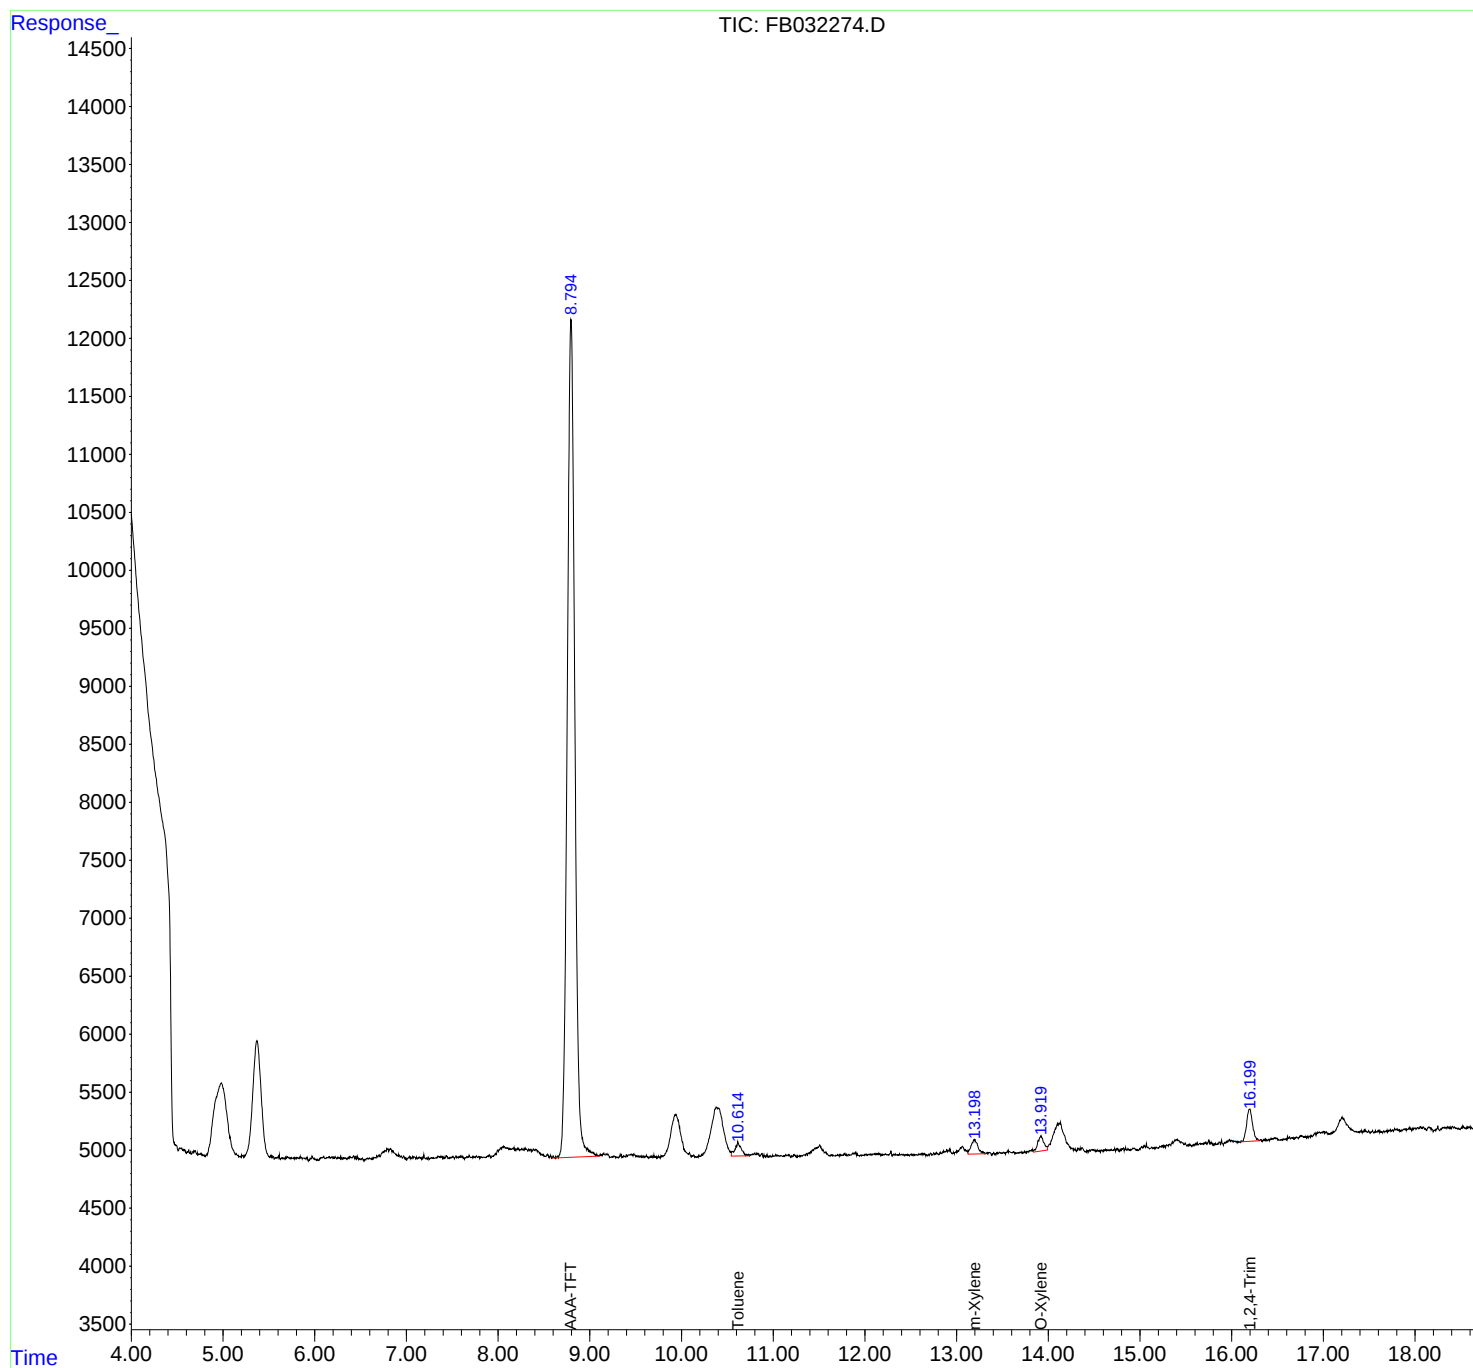


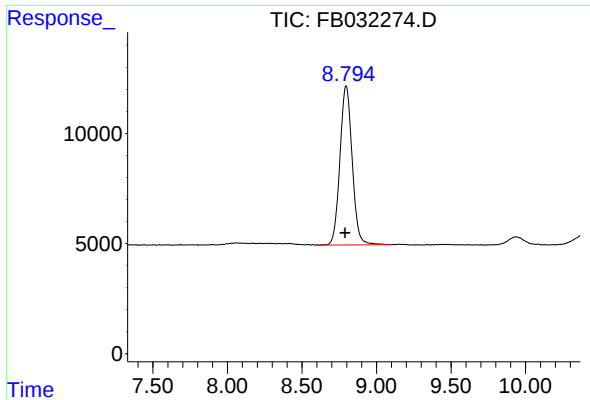

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 412678
Conc: 20.35 ng/ml

Instrument :
FID_E
ClientSampleId :
VBF1103S1

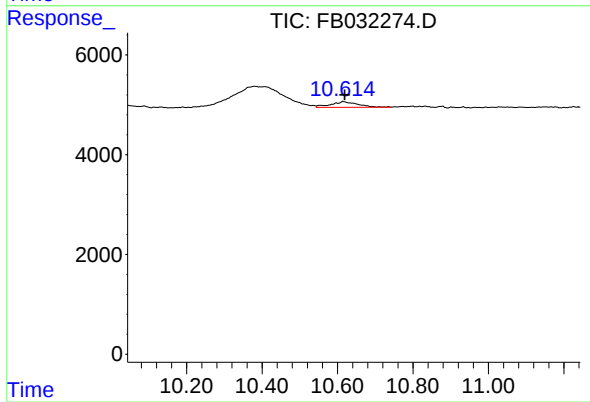


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 5579
Conc: 0.16 ng/ml

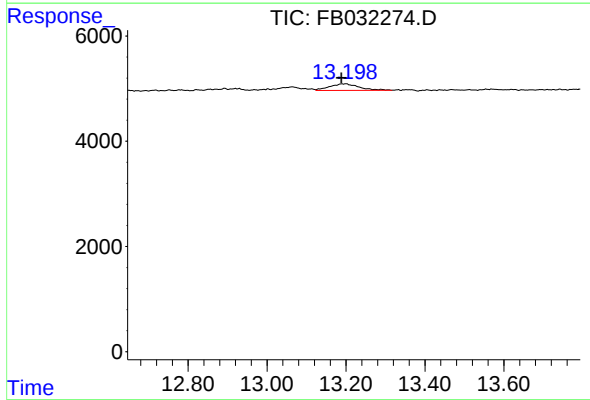


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.012 min
Response: 6329
Conc: 0.19 ng/ml

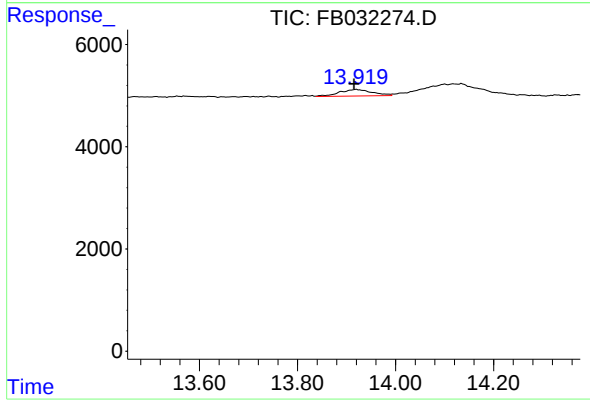

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 6020
Conc: 0.19 ng/ml

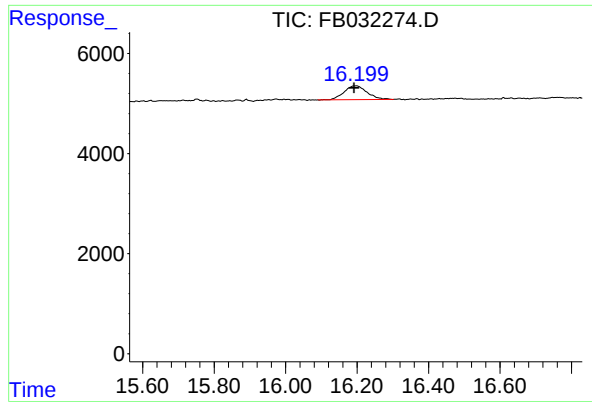

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.007 min
Response: 12430
Conc: 0.45 ng/ml

Instrument :
FID_E
ClientSampleId :
VBF1103S1