

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110325\
 Data File : FB032276.D
 Signal(s) : FID2B.CH
 Acq On : 3 Nov 2025 12:53
 Operator : YP/AJ
 Sample : BSF1103S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 BSF1103S1

Integration File: Calibrat.e
 Quant Time: Nov 04 04:53:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
 Quant Title :
 QLast Update : Tue Oct 28 04:57:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	423358	20.873 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	625873	22.846 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	791156	25.679 ng/ml
3) t n-Heptane	7.756	245173	8.367 ng/ml
4) t Benzene	7.894	329459	9.517 ng/ml
6) t Toluene	10.624	958169	26.779 ng/ml
7) t Ethylbenzene	13.059	284609	8.949 ng/ml
8) t m-Xylene	13.193	595258	17.874 ng/ml
9) t O-Xylene	13.920	589190	18.348 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	492702	17.806 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB110325\
Data File : FB032276.D
Signal(s) : FID2B.CH
Acq On : 3 Nov 2025 12:53
Operator : YP/AJ
Sample : BSF1103S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
BSF1103S1

Integration File: Calibrat.e
Quant Time: Nov 04 04:53:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

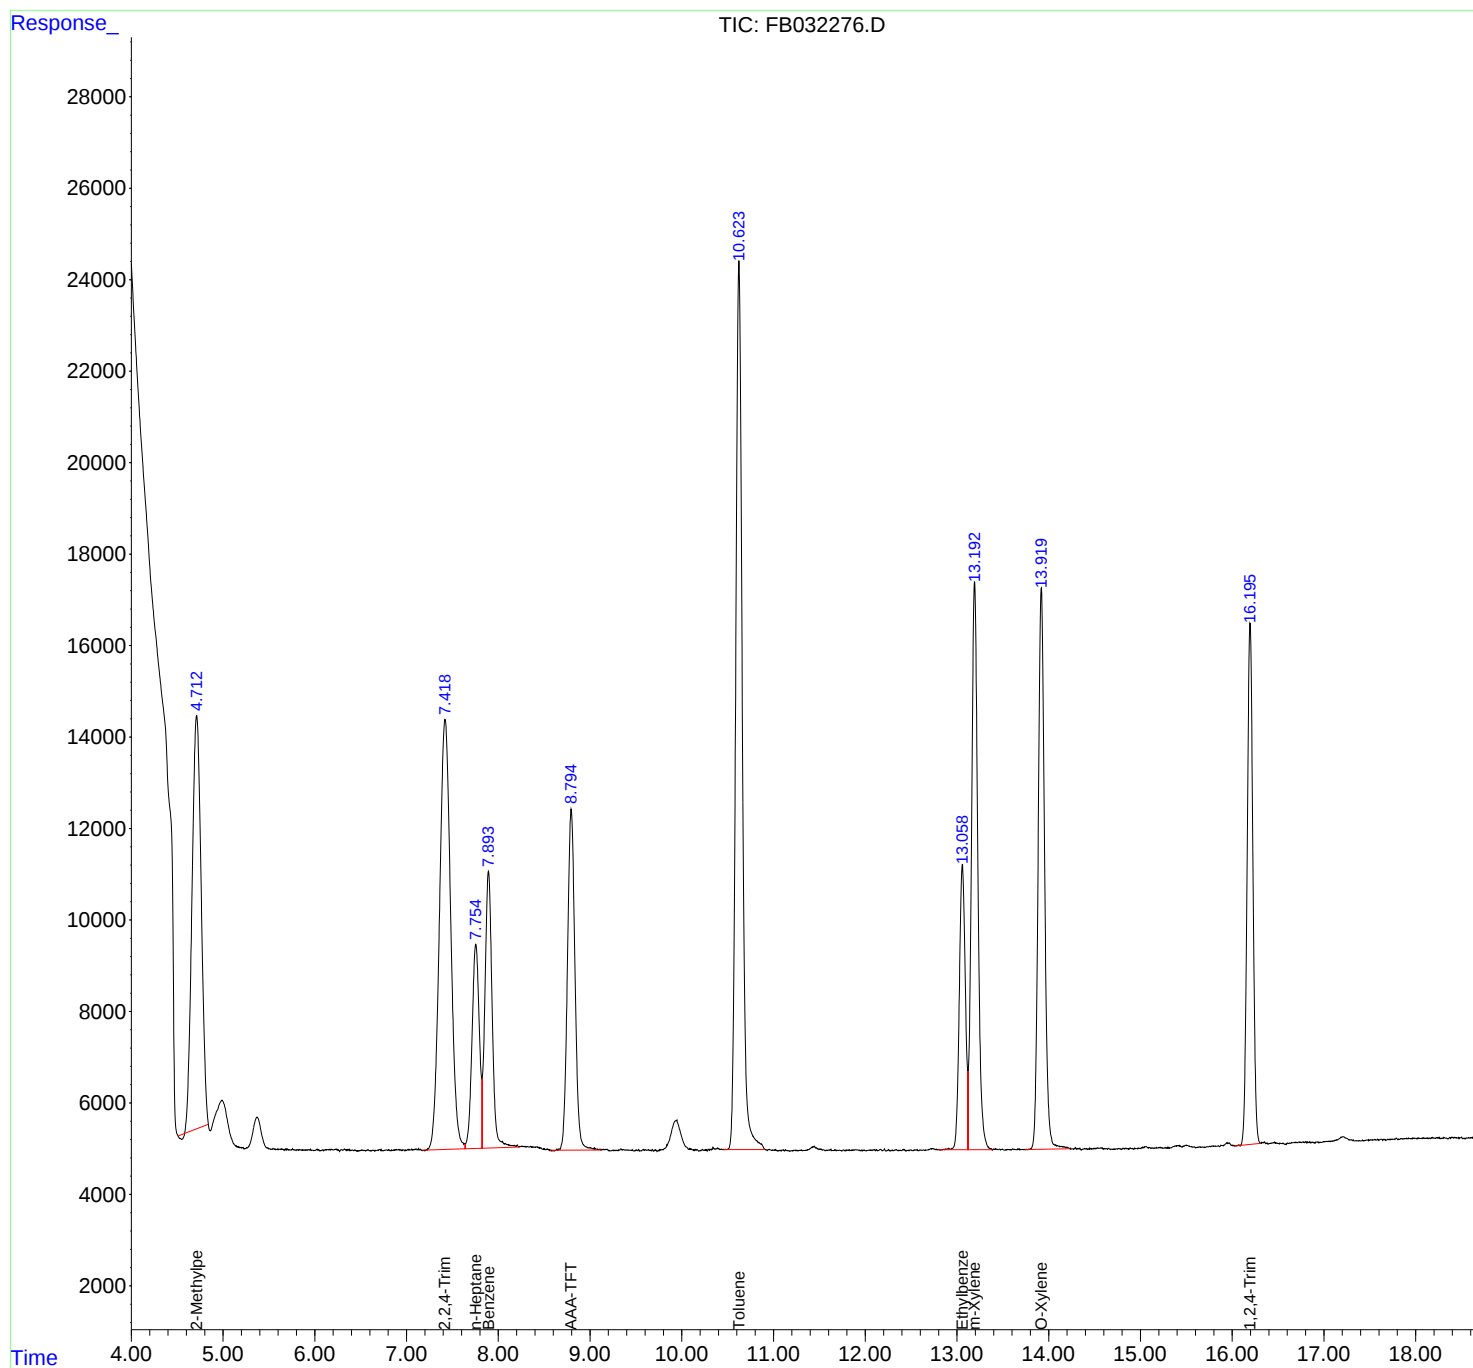


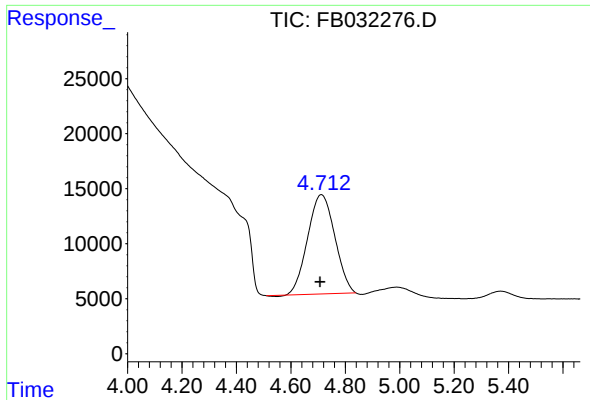

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.006 min
Response: 625873
Conc: 22.85 ng/ml

Instrument :
FID_E
ClientSampleId :
BSF1103S1

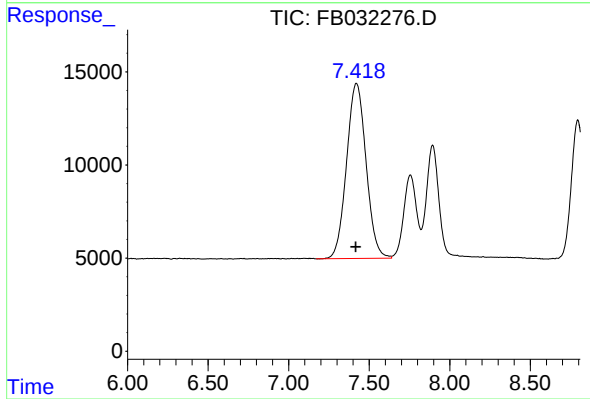


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.004 min
Response: 791156
Conc: 25.68 ng/ml

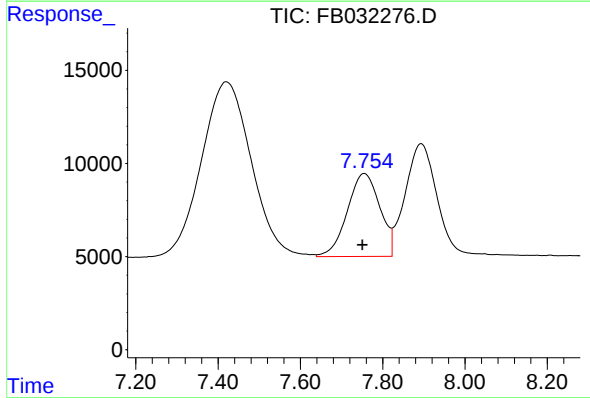


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.005 min
Response: 245173
Conc: 8.37 ng/ml

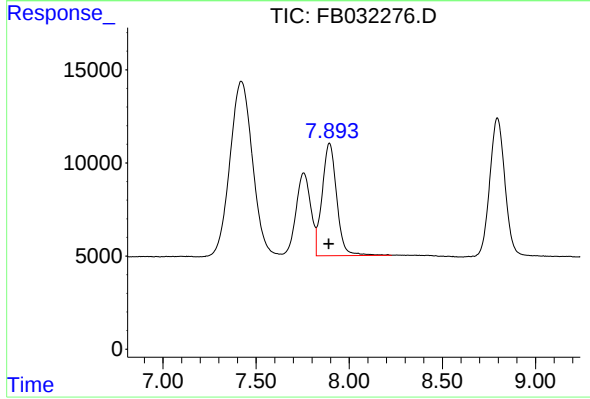

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.005 min
Response: 329459
Conc: 9.52 ng/ml

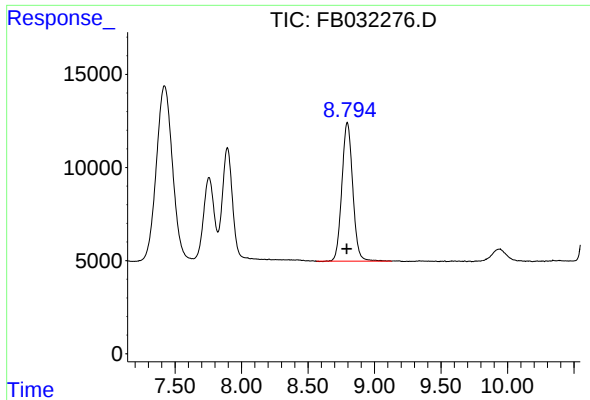

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.005 min
Response: 423358
Conc: 20.87 ng/ml

Instrument :
FID_E
ClientSampleId :
BSF1103S1

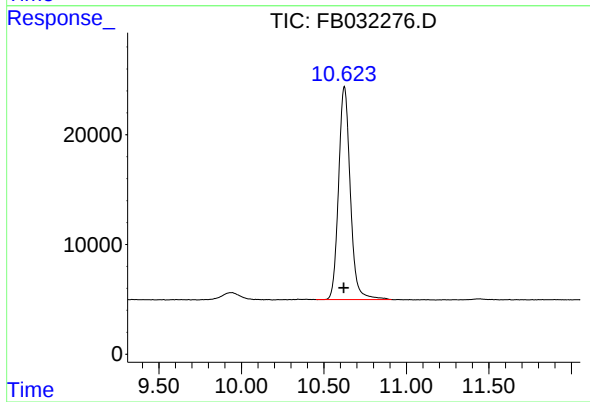


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 958169
Conc: 26.78 ng/ml

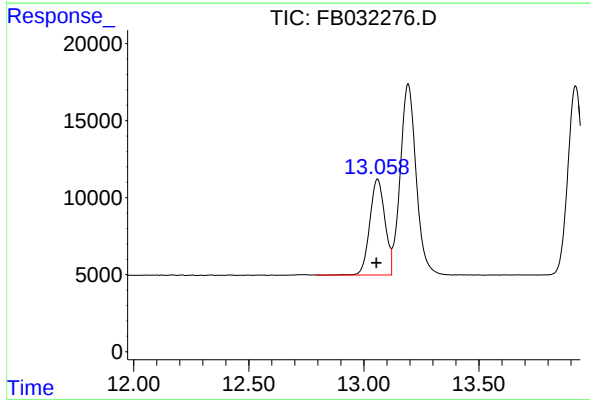


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.004 min
Response: 284609
Conc: 8.95 ng/ml

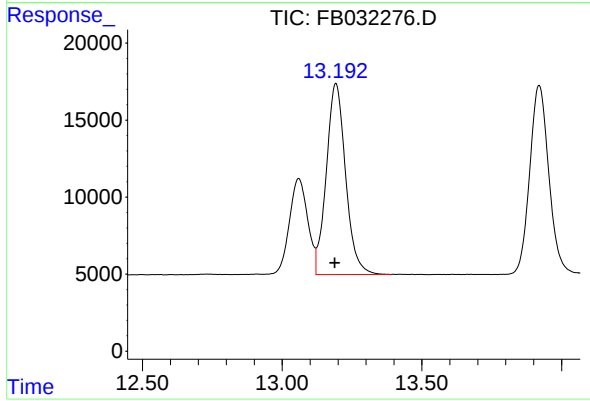

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.004 min
Response: 595258
Conc: 17.87 ng/ml

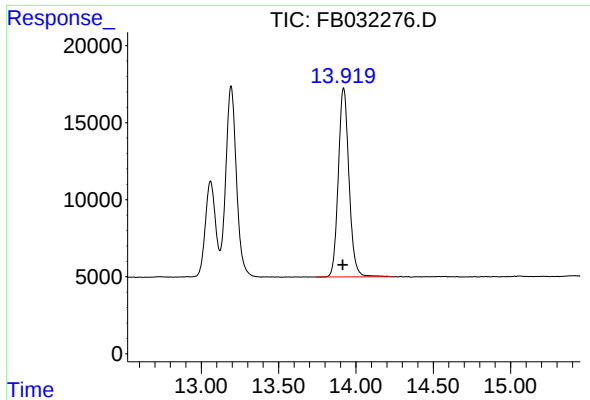

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 589190
Conc: 18.35 ng/ml

Instrument :
FID_E
ClientSampleId :
BSF1103S1

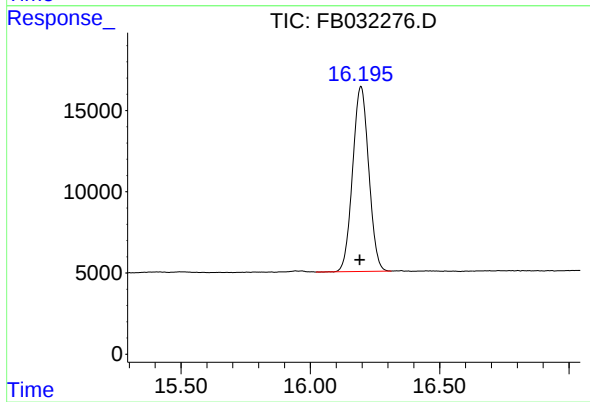

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.005 min
Response: 492702
Conc: 17.81 ng/ml