

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110419\
 Data File : FE030756.D
 Signal(s) : FID1B.CH
 Acq On : 04 Nov 2019 13:51
 Operator : DD\AJ
 Sample : 4400 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 04 14:25:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE110419.M
 Quant Title :
 QLast Update : Mon Nov 04 14:23:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.653	14106755	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.380	102002998	400.000 ug/ml
2) N-NONANE	3.369	102502052	400.000 ug/ml
3) N-DECANE	4.433	154867202	400.000 ug/ml
4) N-UNDECANE	5.466	154658357	600.000 ug/ml
5) N-DODECANE	6.448	153227879	600.000 ug/ml
6) N-TETRADECANE	8.245	152585868	600.000 ug/ml
7) N-HEXADECANE	9.842	125768770	500.000 ug/ml
8) N-OCTADECANE	11.267	61905287	250.000 ug/ml
9) N-EICOSANE	12.560	24207012	100.000 ug/ml
10) N-TETRACOSANE	14.653	14106755	100.000 ug/ml
11) N-OCTACOSANE	16.823	11453240	50.000 ug/ml
12) N-DOTRIACONTANE	18.542	9989314	50.000 ug/ml
14) N-HEXATRIACONTANE	20.063	8308818	50.000 ug/ml
15) N-TETRACONTANE	21.685	7107598	50.000 ug/ml
16) N-TETRTETRACOOCTANE	24.403	4598814	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110419\
Data File : FE030756.D
Signal(s) : FID1B.CH
Acq On : 04 Nov 2019 13:51
Operator : DD\AJ
Sample : 4400 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 04 14:25:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE110419.M
Quant Title :
QLast Update : Mon Nov 04 14:23:59 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

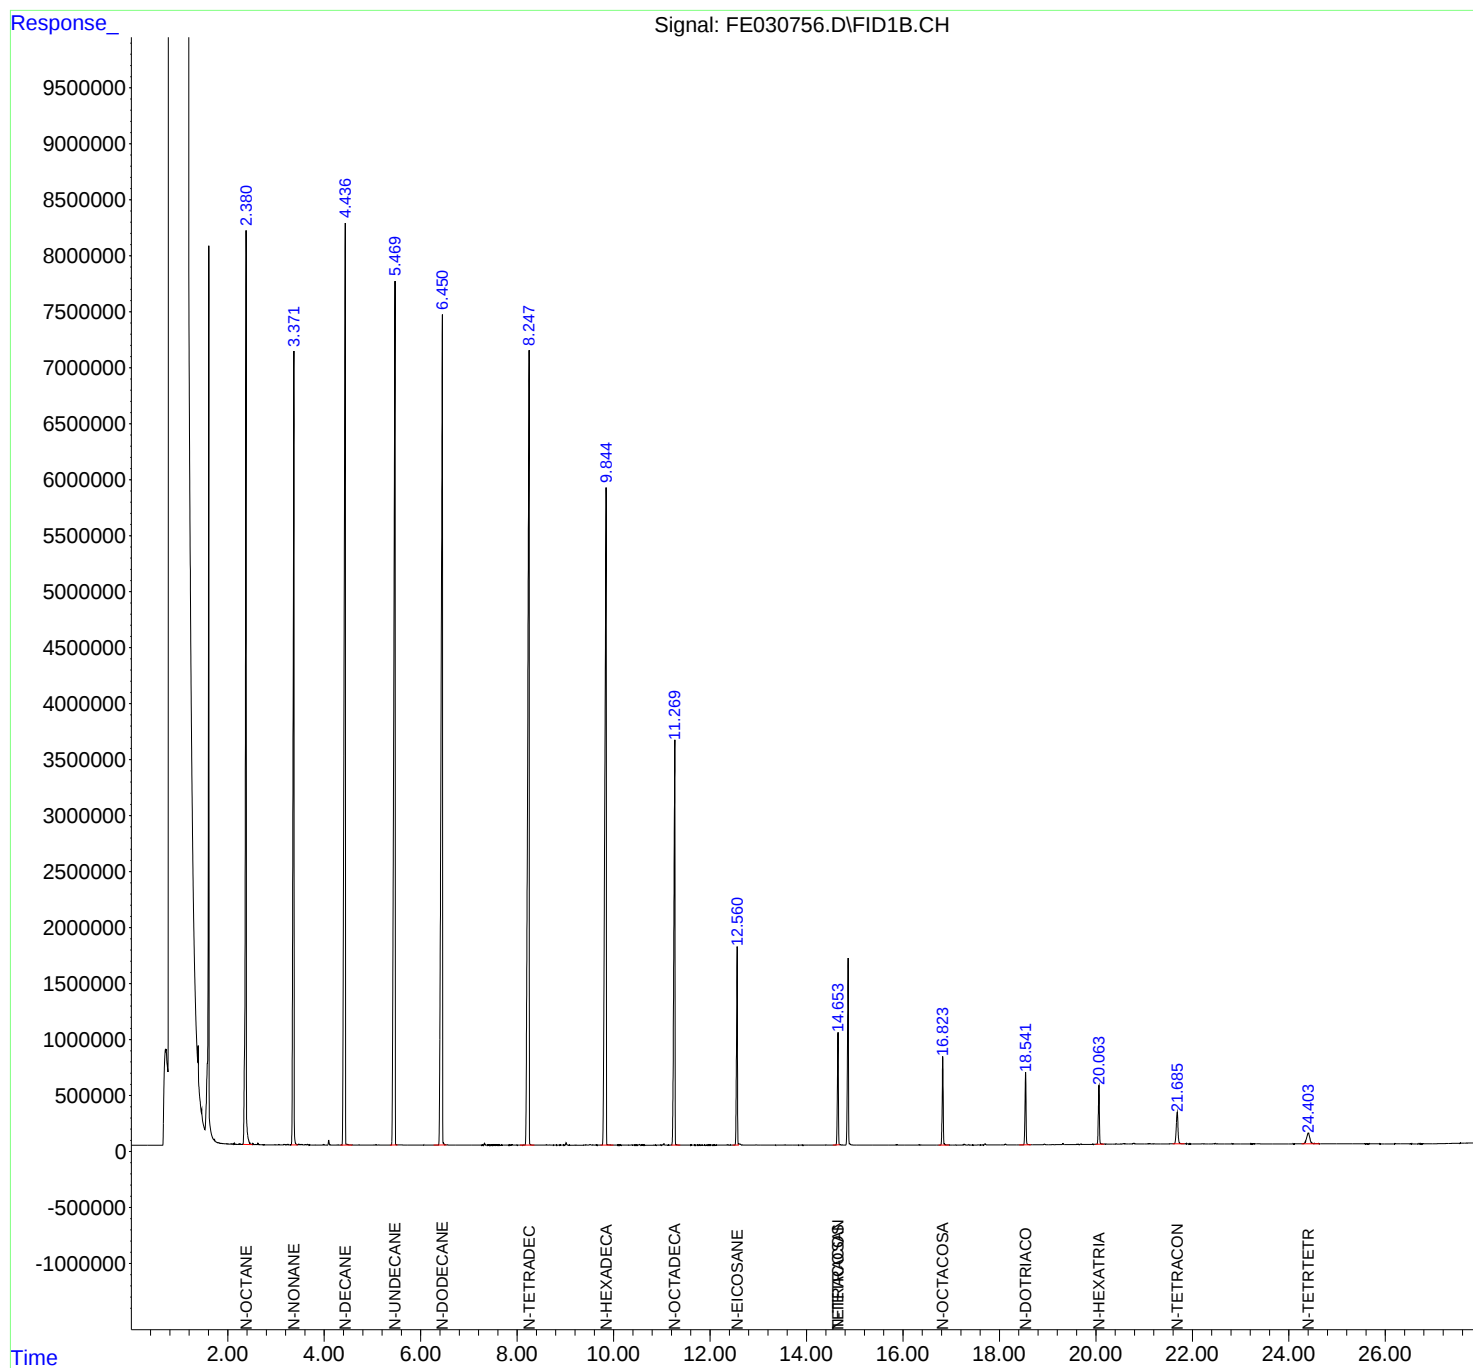

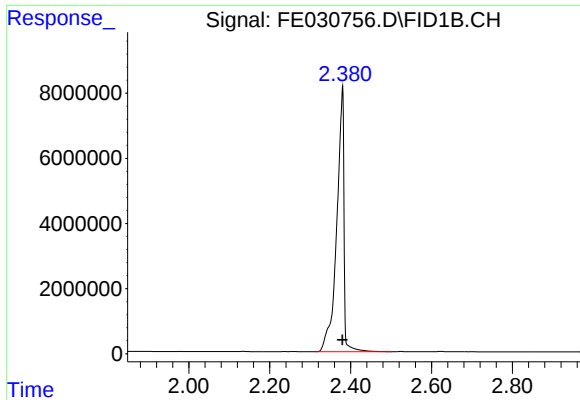


#1 N-OCTANE

R.T.: 2.380 min
Delta R.T.: 0.000 min
Response: 102002998
Conc: 400.00 ug/ml

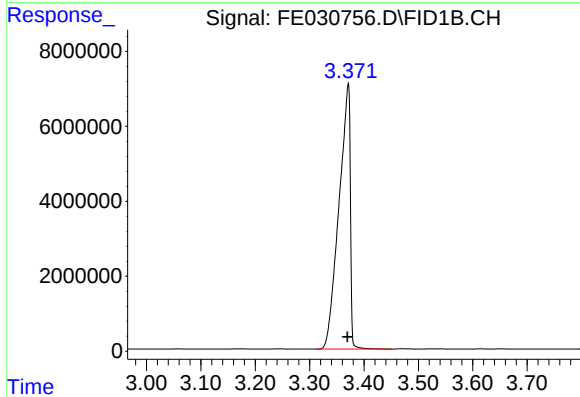


#2 N-NONANE

R.T.: 3.369 min
Delta R.T.: 0.000 min
Response: 102502052
Conc: 400.00 ug/ml

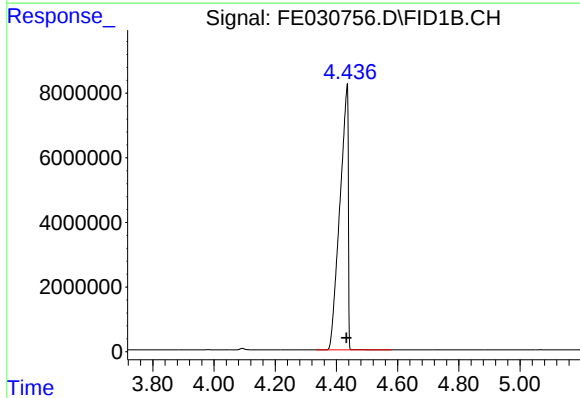


#3 N-DECANE

R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 154867202
Conc: 400.00 ug/ml

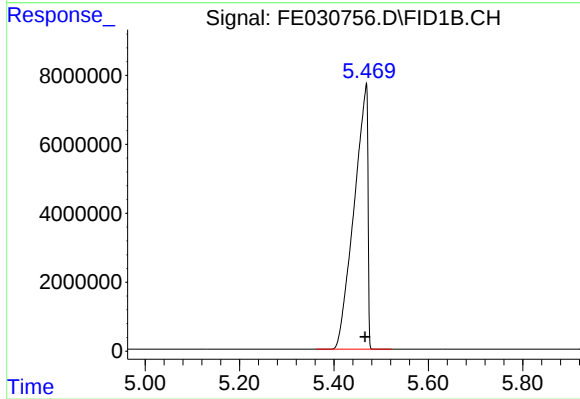


#4 N-UNDECANE

R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 154658357
Conc: 600.00 ug/ml

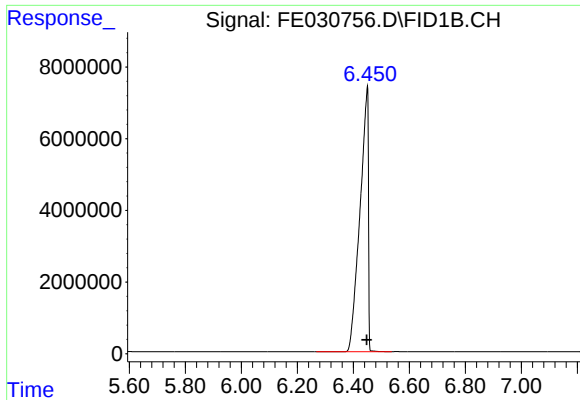


#5 N-DODECANE

R.T.: 6.448 min
Delta R.T.: 0.000 min
Response: 153227879
Conc: 600.00 ug/ml

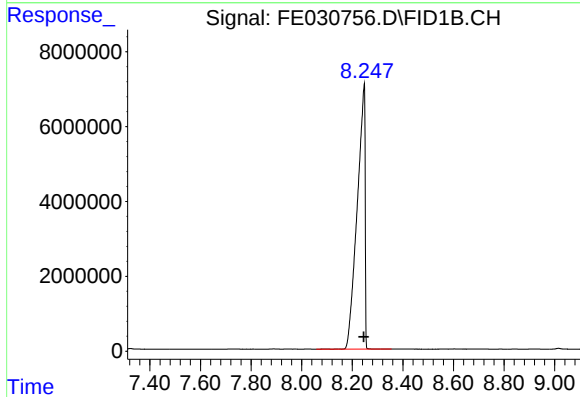


#6 N-TETRADECANE

R.T.: 8.245 min
Delta R.T.: 0.000 min
Response: 152585868
Conc: 600.00 ug/ml

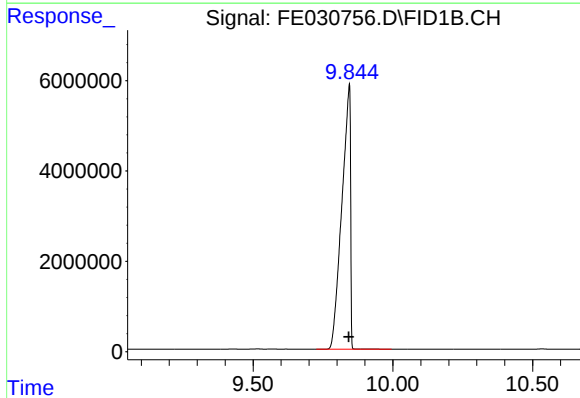


#7 N-HEXADECANE

R.T.: 9.842 min
Delta R.T.: 0.000 min
Response: 125768770
Conc: 500.00 ug/ml

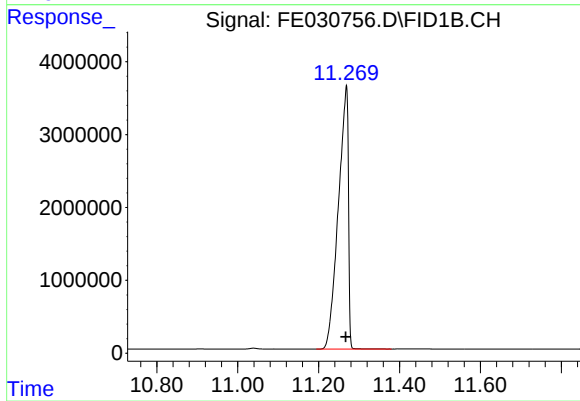


#8 N-OCTADECANE

R.T.: 11.267 min
Delta R.T.: 0.000 min
Response: 61905287
Conc: 250.00 ug/ml

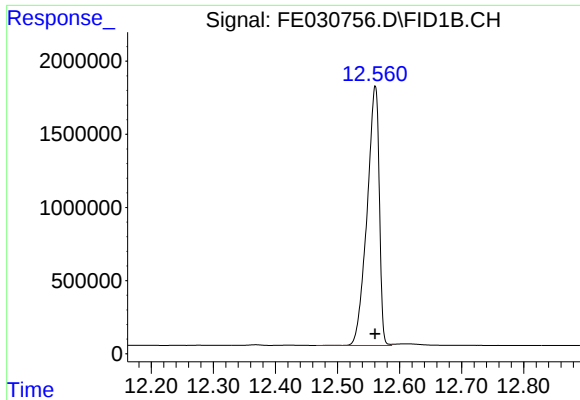


#9 N-EICOSANE

R.T.: 12.560 min
Delta R.T.: 0.000 min
Response: 24207012
Conc: 100.00 ug/ml

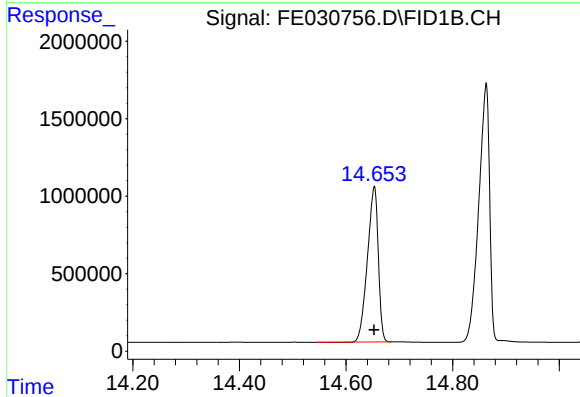


#10 N-TETRACOSANE

R.T.: 14.653 min
Delta R.T.: 0.000 min
Response: 14106755
Conc: 100.00 ug/ml

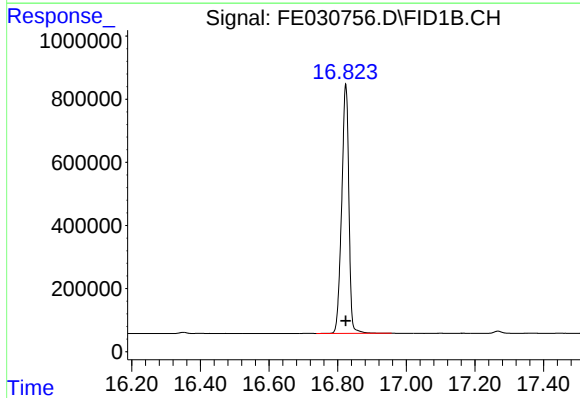


#11 N-OCTACOSANE

R.T.: 16.823 min
Delta R.T.: 0.000 min
Response: 11453240
Conc: 50.00 ug/ml

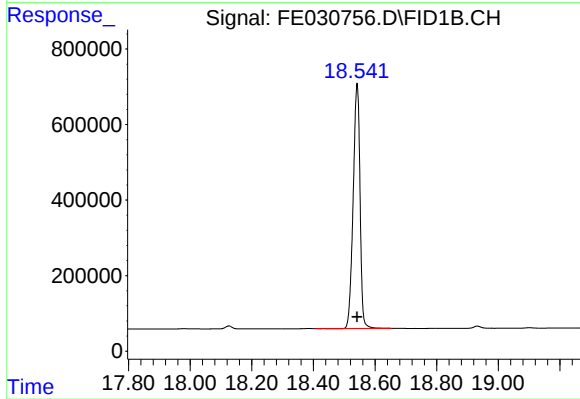


#12 N-DOTRIACONTANE

R.T.: 18.542 min
Delta R.T.: 0.000 min
Response: 9989314
Conc: 50.00 ug/ml

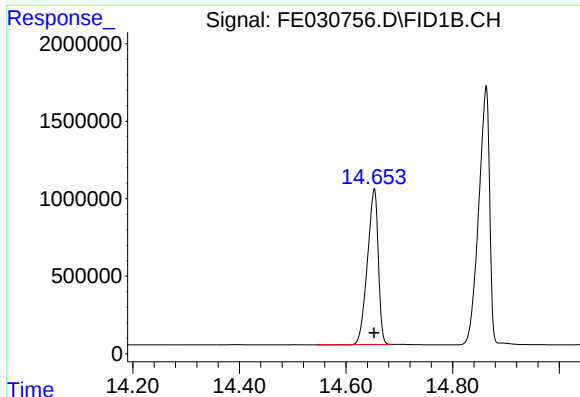


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.653 min
Delta R.T.: 0.000 min
Response: 14106755
Conc: 50.00 ug/ml

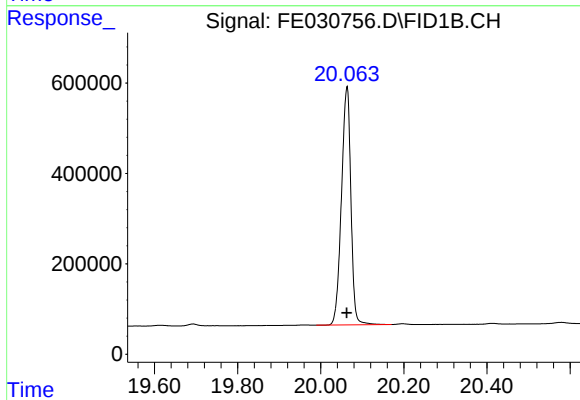


#14 N-HEXATRIACONTANE

R.T.: 20.063 min
Delta R.T.: 0.000 min
Response: 8308818
Conc: 50.00 ug/ml

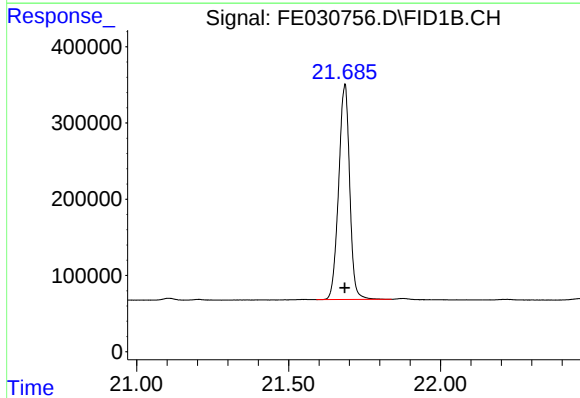

#15 N-TETRACONTANE

R.T.: 21.685 min
Delta R.T.: 0.000 min
Response: 7107598
Conc: 50.00 ug/ml

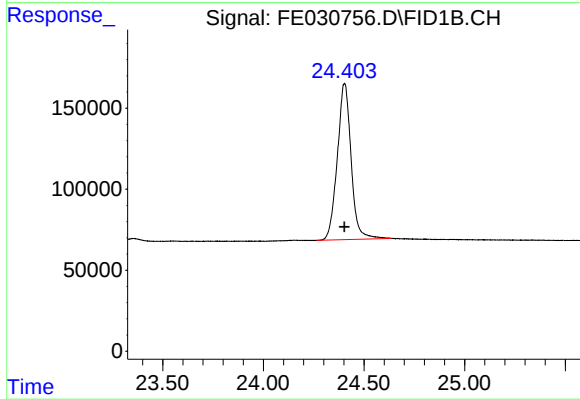

#16 N-TETRTETRACOOCTANE

R.T.: 24.403 min
Delta R.T.: 0.000 min
Response: 4598814
Conc: 50.00 ug/ml