

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110518\
 Data File : FE028997.D
 Signal(s) : FID1B.CH
 Acq On : 05 Nov 2018 17:55
 Operator : DD\SJ
 Sample : J5805-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 06 08:13:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE102518.M
 Quant Title :
 QLast Update : Thu Oct 25 04:58:05 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.926	2045549	11.888 ug/ml
Target Compounds			
7) N-EICOSANE	12.816	287987	1.431 ug/ml
8) N-DOCOSANE	14.017	169101	0.843 ug/ml
10) N-TETRACOSANE	15.113	1740052	8.962 ug/ml
11) N-HEXACOSANE	16.128	306368	1.627 ug/ml
12) N-OCTACOSANE	17.092	1456538	7.988 ug/ml
13) N-TRIACONTANE	17.944	575464	3.233 ug/ml
14) N-DOTRIACONTANE	18.857	1786651	10.191 ug/ml
15) N-TETRATRIACONTANE	19.651f	509270	2.891 ug/ml
16) N-HEXATRIACONTANE	20.344	1235079	6.968 ug/ml
17) N-OCTATRIACONTANE	21.198f	392668	2.424 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110518\
Data File : FE028997.D
Signal(s) : FID1B.CH
Acq On : 05 Nov 2018 17:55
Operator : DD\SJ
Sample : J5805-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 06 08:13:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE102518.M
Quant Title :
QLast Update : Thu Oct 25 04:58:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

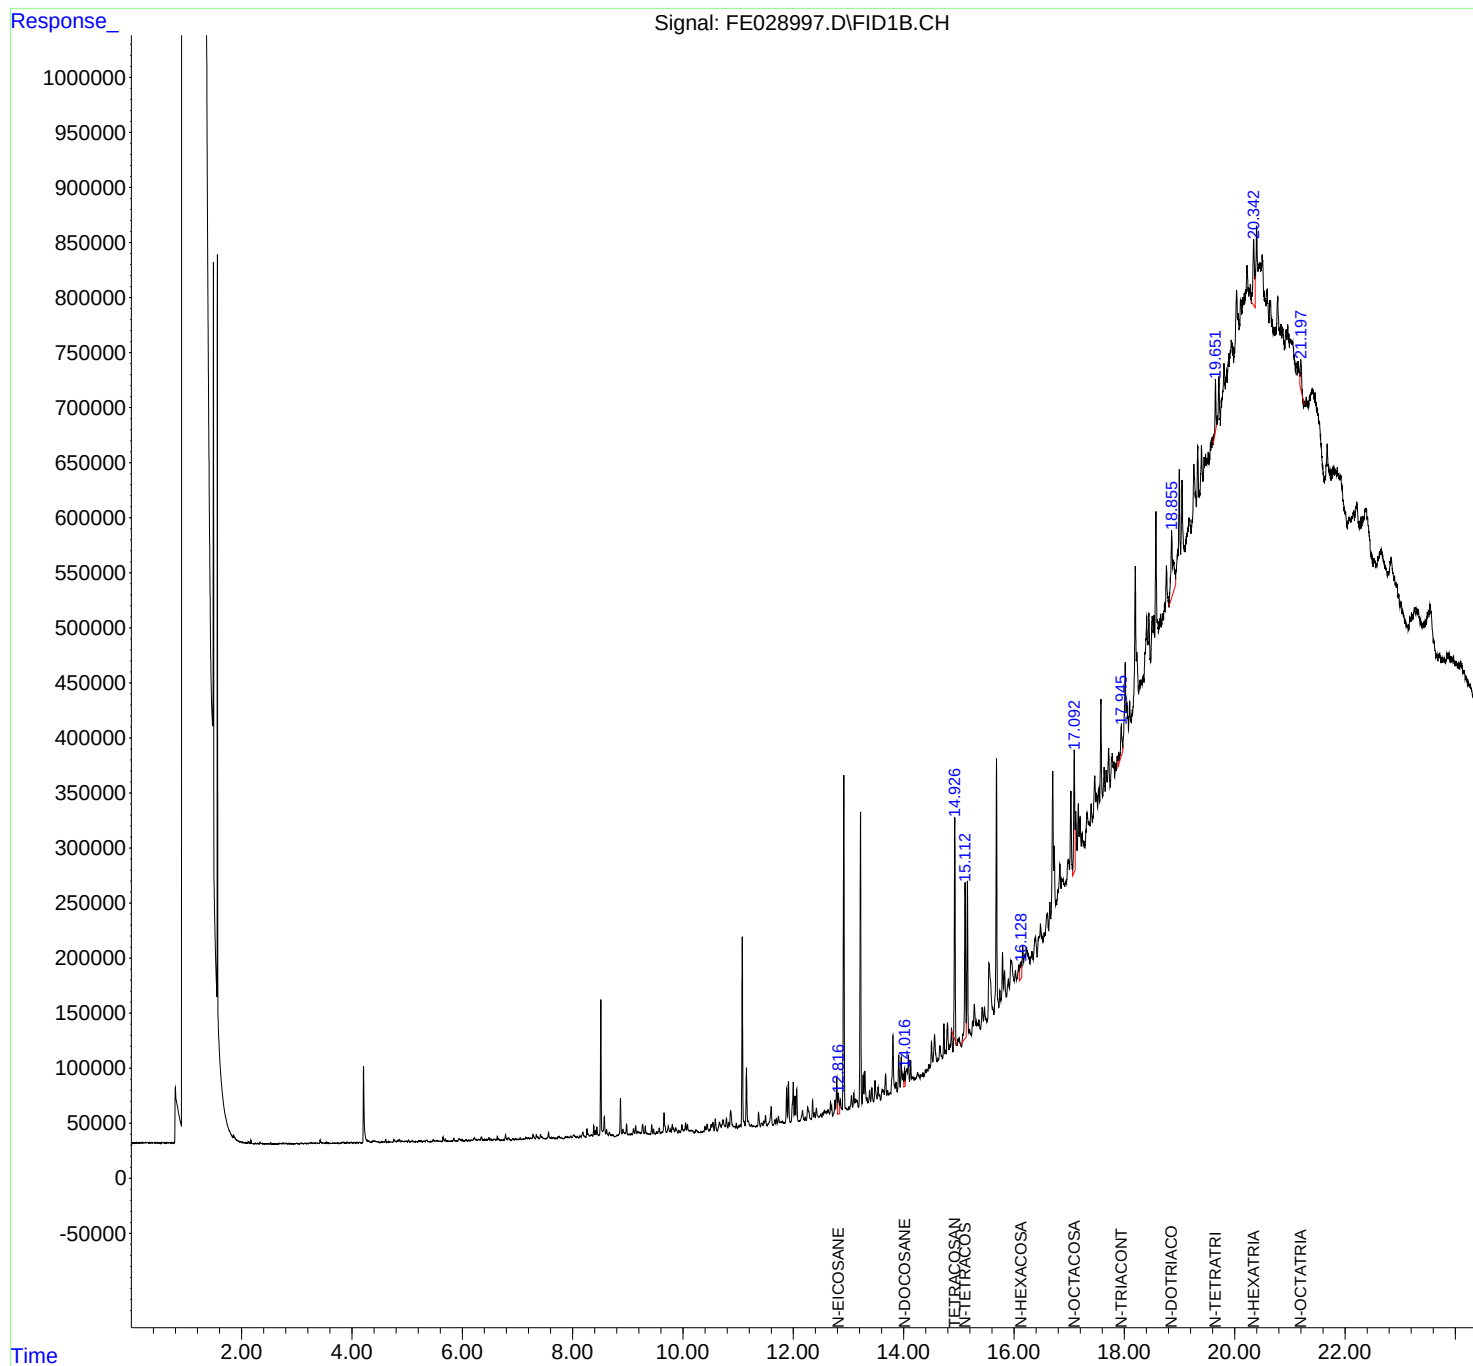

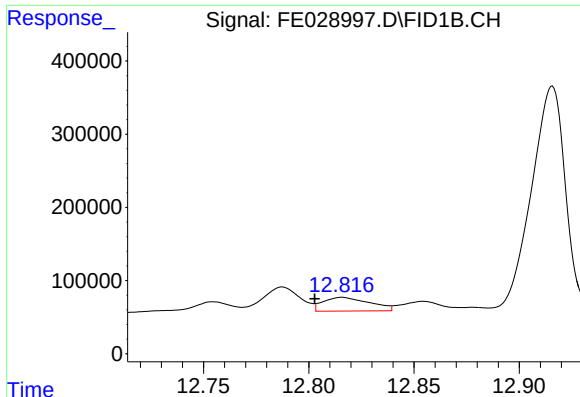


#7 N-EICOSANE

R.T.: 12.816 min
Delta R.T.: 0.013 min
Response: 287987
Conc: 1.43 ug/ml

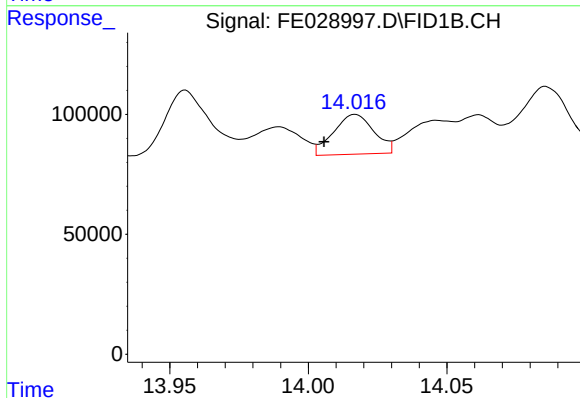


#8 N-DOCOSANE

R.T.: 14.017 min
Delta R.T.: 0.011 min
Response: 169101
Conc: 0.84 ug/ml

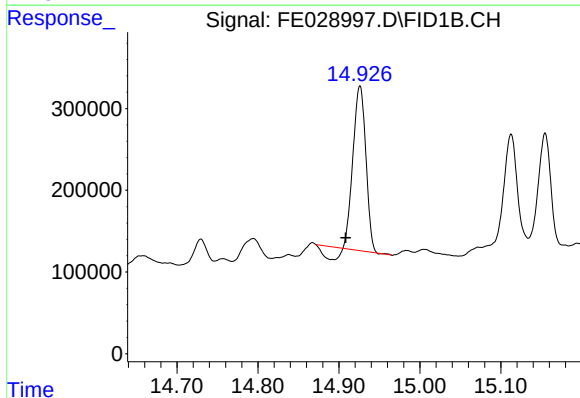


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.926 min
Delta R.T.: 0.017 min
Response: 2045549
Conc: 11.89 ug/ml

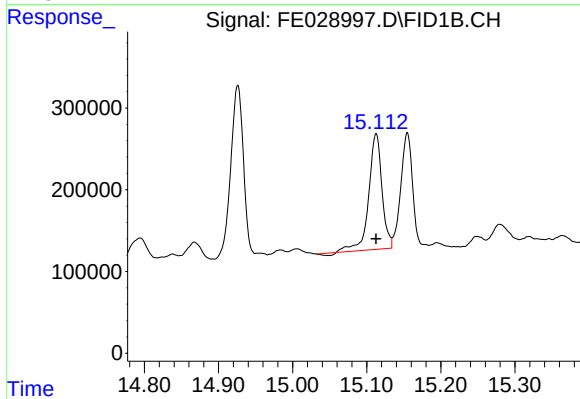


#10 N-TETRACOSANE

R.T.: 15.113 min
Delta R.T.: 0.000 min
Response: 1740052
Conc: 8.96 ug/ml

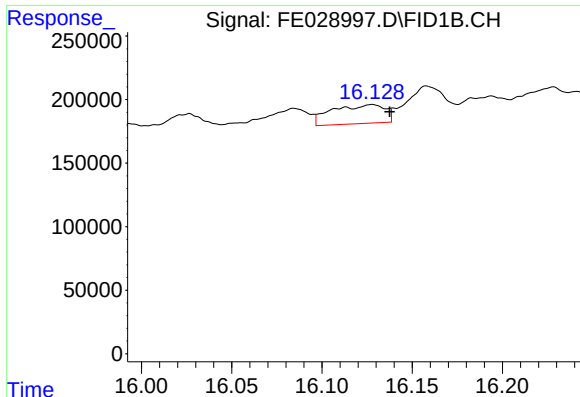


#11 N-HEXACOSANE

R.T.: 16.128 min
Delta R.T.: -0.010 min
Response: 306368
Conc: 1.63 ug/ml

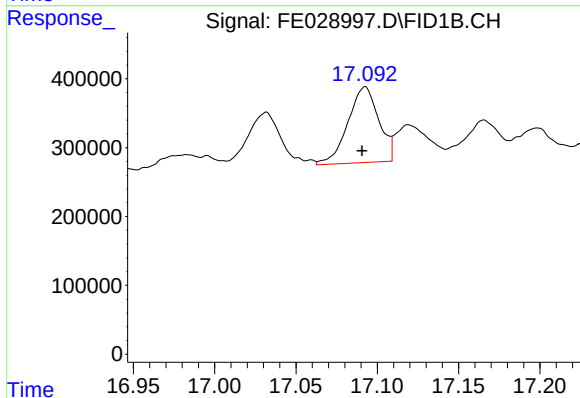


#12 N-OCTACOSANE

R.T.: 17.092 min
Delta R.T.: 0.002 min
Response: 1456538
Conc: 7.99 ug/ml

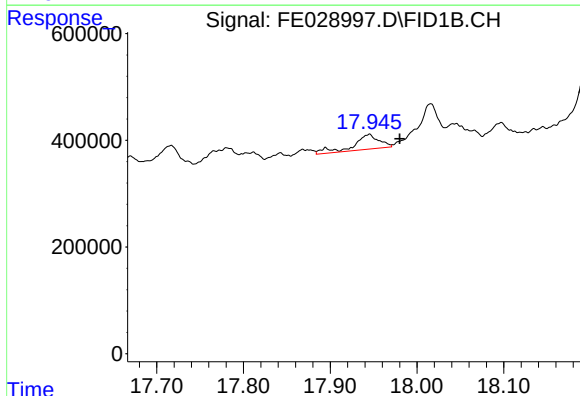


#13 N-TRIACONTANE

R.T.: 17.944 min
Delta R.T.: -0.036 min
Response: 575464
Conc: 3.23 ug/ml

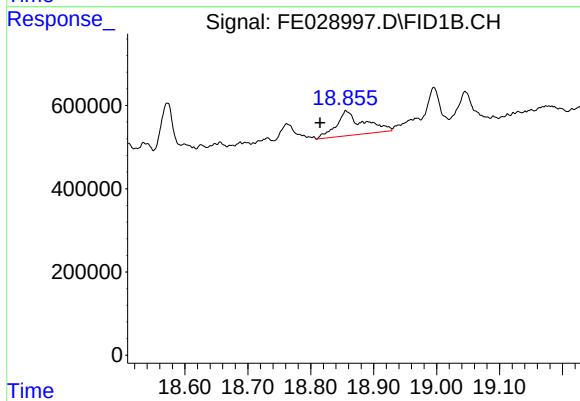


#14 N-DOTRIACONTANE

R.T.: 18.857 min
Delta R.T.: 0.042 min
Response: 1786651
Conc: 10.19 ug/ml

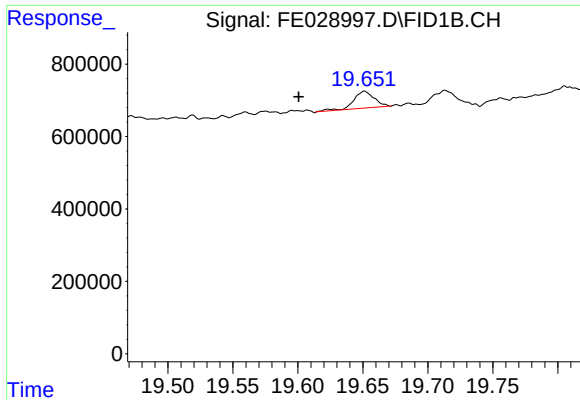


#15 N-TETRATRIACONTANE

R.T.: 19.651 min
Delta R.T.: 0.051 min
Response: 509270
Conc: 2.89 ug/ml

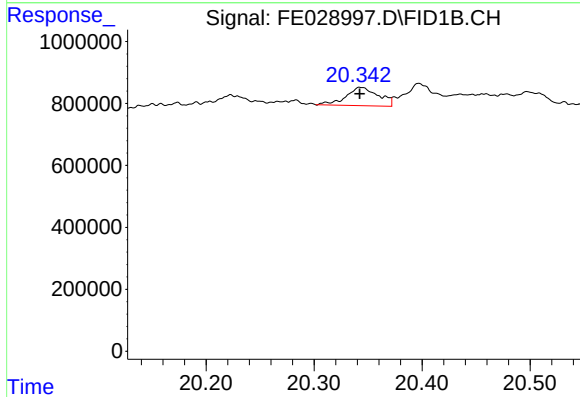

#16 N-HEXATRIACONTANE

R.T.: 20.344 min
Delta R.T.: 0.001 min
Response: 1235079
Conc: 6.97 ug/ml

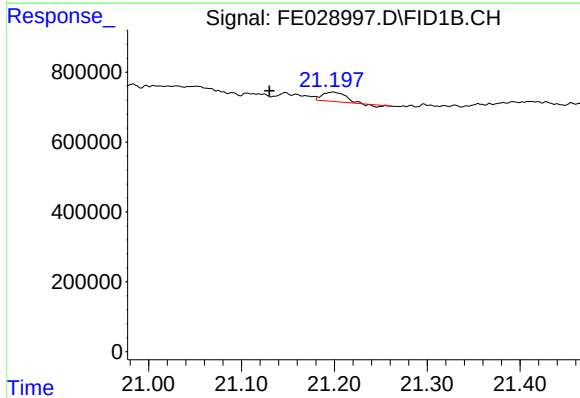

#17 N-OCTATRIACONTANE

R.T.: 21.198 min
Delta R.T.: 0.068 min
Response: 392668
Conc: 2.42 ug/ml